


Contents lists available at [ScienceDirect](https://www.sciencedirect.com)

Journal of Advanced Research

journal homepage: www.elsevier.com/locate/jareEmerging analytical tools for the detection of the third gasotransmitter H₂S, a comprehensive reviewHany Ibrahim^{a,1}, Ahmed Serag^{b,1}, Mohamed A. Farag^{c,d,*}^a Analytical Chemistry Department, Faculty of Pharmacy, Egyptian Russian University, Cairo 11829, Egypt^b Pharmaceutical Analytical Chemistry Department, Faculty of Pharmacy, Al-Azhar University, Cairo 11751, Egypt^c Pharmacognosy Department, Faculty of Pharmacy, Cairo University, Cairo 11562, Egypt^d Department of Chemistry, School of Sciences & Engineering, The American University in Cairo, New Cairo 11835, Egypt

GRAPHICAL ABSTRACT

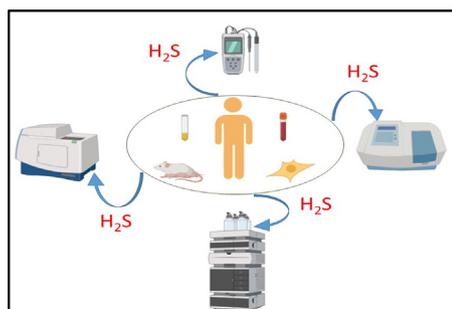

ARTICLE INFO

Article history:

Received 4 April 2020

Revised 15 May 2020

Accepted 15 May 2020

Available online 25 May 2020

Keywords:

Hydrogen sulfide H₂S

in vivo detection

Fluorescent probes

Colorimetric probes

Chemiluminescent probes

Chromatographic bioanalysis

Chromatographic methods

Electrochemical sensors

ABSTRACT

Background: Hydrogen sulfide (H₂S) is currently considered among the endogenously produced gaseous molecules that exert various signaling effects in mammalian species. It is the third physiological gasotransmitter discovered so far after NO and CO. H₂S was originally ranked among the toxic gases at elevated levels to humans. Currently, it is well-known that, in the cardiovascular system, H₂S exerts several cardioprotective effects including vasodilation, antioxidant regulation, inhibition of inflammation, and activation of anti-apoptosis. With an increasing interest in monitoring H₂S, the development of analysis methods should now follow.

Aim of review: This review stages special emphasis on the several analytical technologies used for its determination including spectroscopic, chromatographic, and electrochemical methods. Advantages and limitations with regards to the application of each technique are highlighted with special emphasis on its employment for H₂S *in vivo* measurement *i.e.*, biofluids, tissues.

Key Scientific Concepts and important findings of Review: Fluorescence methods applied for H₂S measurement offer an attractive non-invasive and promising approach in addition to its selectivity, however they cannot be considered as H₂S-specific probes. On the other hand, colorimetric assays are among the most common methods used for *in vitro* H₂S detection, albeit their employment *in vivo* H₂S measurement has not yet been possible. Separation techniques such as gas or liquid chromatography offer higher selectivity compared to direct spectrophotometric or fluorescence methods especially for suitable for endpoint H₂S measurements *i.e.* plasma or tissue samples. Despite all the developed analytical procedures used

Peer review under responsibility of Cairo University.

* Corresponding author.

E-mail address: Mohamed.farag@pharma.cu.edu.eg (M.A. Farag).¹ Contributed equally.<https://doi.org/10.1016/j.jare.2020.05.018>

2090-1232/© 2020 The Authors. Published by Elsevier B.V. on behalf of Cairo University.

This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

for H₂S determination, the need for highly selective, much work should be devoted to resolve all the pitfalls of the current methods.

© 2020 The Authors. Published by Elsevier B.V. on behalf of Cairo University. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

Introduction

Hydrogen sulfide (H₂S) is an important gaseous signaling molecule that sits with nitric oxide and carbon monoxide as the biologically active family of “gaseous mediators” or “gasotransmitters” [1]. It is produced at low concentrations in mammalian systems mainly *via* enzymatic interconversions of sulfur-containing substrates to fulfill a vast number of biological functions in almost every organ [2]. For example, in the central nervous system it acts as a neuromodulator [3] in addition to its effect for controlling perception of pain and neuronal potentiation [4]. In the cardiovascular system, it causes vasodilation and protects vasculature from reperfusion injury [5,6]. Besides, H₂S plays other pivotal biological roles *viz.*, angiogenesis, anti-inflammation, inhibition of insulin signaling, regulation of blood pressure [7], and even involved in longevity [8]. On the other hand, H₂S also participates in many pathological activities of various diseases, such as Parkinson’s disease [9], Alzheimer’s disease [10], Down’s syndrome [11] and diabetes [12]. Owing to its vast involvement in various physiological processes, H₂S-based therapeutics have been recently investigated [1]. Consequently, it is of great importance to develop fast and sensitive determination methods to scrutinize H₂S levels. However, *in vivo* monitoring and detection of H₂S faces many serious challenges owing to its promiscuous chemical properties such as volatility, high reactivity, and rapid catabolism. Besides, H₂S presents, under physiological conditions, pH 7.4 and 37 °C, in different chemical ionization forms *i.e.* approximately 18.5% H₂S, 81.5% hydrosulfide anion (HS⁻) and a negligible contribution of S²⁻ [13]. Moreover, it might also exist in different bound forms such as acid-, base-labile and reducible forms, which are utilized in liberating free hydrogen sulfide following physiological stimuli in biological systems [14]. In addition, the extraction and sample treatment of H₂S may face interference from the biological matrices such as proteins present in blood, plasma, serum and cells [15,16] thus the real concentration of H₂S in different biological samples was in debate for a long time due to the disaccording reported data [17].

Owing to the previously mentioned challenges for H₂S determination, developed analytical methodologies should fulfill certain criteria to be successfully implemented including sufficient sensitivity for endogenous H₂S, real-time monitoring for H₂S level changes and high selectivity for H₂S over other endogenous biothiols (*ex.* glutathione, cysteine ...) or other ions present in the blood or tissues under investigation. Hence, a plethora of different analytical methods has evolved for H₂S measurements such as fluorescence-based assays [18], colorimetric sensors [19], chromatographic methods (HPLC and GC) [20] and electrochemical methods (ion-selective electrodes and polarographic H₂S sensors) [21]. However, each of these techniques has its advantages and limitations. Colorimetric and chromatographic assays have been used for the bulk measurement of both plasma and tissue H₂S, however, they do not have the capability for real-time monitoring of H₂S within intact tissues or living cells, in addition, they are denounced to be sample-destructive. On the other hand, fluorescence-based sensors have been developed to meet these challenges and to provide sensitive and biocompatible detection tools for H₂S not only within certain tissues but also within subcellular organelles. Ion selective electrodes have also been widely used as an effective method to measure the H₂S in different biological matrices with distinct advantages of low detection limit and fast response, however, vigorous alkaline conditions are required

to convert H₂S and HS⁻ to S²⁻ as this is the only form the electrode can measure. Unfortunately, liberation of sulfur from other biomolecules has been detected at such conditions which could lead to an overestimation of molecular H₂S concentrations.

Several reviews have reported on the different analytical approaches applied for the determination of this gaseous signaling molecule [18,22–28]. However, most of these reviews focused only on spectroscopic techniques with special emphasis on probe materials [18,19,29], design strategies [27,30], and detection mechanisms [28,31]. Besides, very few reports have discussed other analytical methodologies such as electrochemical and chromatographic methods [21,22]. In this review, we summarize the information about the currently available state-of-the-art analytical techniques used to measure physiological H₂S levels. The reported methods were organized into categories following their instrumentation type and then subdivided based on their working principle. Also, the advantages and limitations of these methods have been addressed to guide researchers through the appropriate analytical tool to choose for their application.

Fluorescence-based sensors

While chromatographic assays and electrochemical sensors have been used to determine H₂S levels in the blood, homogenized tissues, and cell lysates [32], these methods are mostly less suited for its determination in living biological specimens. Though, fluorescence techniques have attracted much attention as sensors offering excellent sensitivity, good selectivity, rapid response, and non-invasive detection with a high spatiotemporal resolution for both *in vitro* and *in vivo* imaging as typically needed for quantifying H₂S. Moreover, fluorescence-based sensors offer real-time H₂S monitoring not only within certain tissues but also within subcellular organelles. Therefore, the evolution of H₂S- fluorescence probes is considered one of the most rapid-growing areas in the field of H₂S biology [17]. Though, a substantial increase in the number of developed small molecule-based sensors was remarked in the past decade. Diverse small organic compounds and metal chelates have been explored with different H₂S-reaction sites. Recently, nanotechnology was implemented for the development of effective and highly sensitive fluorescent nanosensors used for H₂S detection [33] as typical in the detection of other signaling molecules or drugs.

Monitoring H₂S in subcellular structures is considered crucial for biomarkers discovery and related drug discovery. Therefore, the emergence of organelle-targeted fluorescent probes is essential for subcellular imaging revealing the physiological and pathological functions of these highly reactive, interactive, and interconvertible molecules during diverse biological events, which are significant for the understanding of diseases etiology. Organelle-targeted fluorescent probes should encompass three moieties: targeting groups, fluorophores, and recognition units. Many cellular organelles-targeting scaffolds were coupled with the fluorophore and the H₂S-recognition moieties. For example, the mitochondrial-targeting entities comprise positively charged groups as triphenylphosphonium, quaternary ammonium, isoquinolinium, acridine, indolium, and pyridium [34]. Whereas the sulfide-recognition entities include azides, nitro, hydroxylamine, dinitrophenyl, NBD. After reaching subcellular locations of interest, probes can subsequently react with free sulfide through and specific reaction mechanisms and consequently fluorescence response

measurements *via* turn-on, -off, or ratiometric, which enables the monitor of targeted species in different organelles [35,36].

The determination of endogenous H₂S *in vivo* presents indeed many challenges due to its low concentration, short half-life time with fast catabolism, and high reactivity. Although there are limits of measurement techniques and the quantification of biological H₂S levels is debated, H₂S physiological levels may range from 50 to 160 μM in the mammalian brain, to 30 nM–100 μM in the peripheral blood, 25 μM in the synovial fluid of non-inflammatory arthritic patients [37], 8.9 nM in mice liver tissue [38]. An ideal fluorescent probe should thus fulfill the following criteria:

- i) to be sufficiently sensitive for endogenous H₂S detection and real-time monitoring for the changes in H₂S fluxes in living cells,
- ii) to react rapidly (spontaneously) under physiological conditions (*i.e.*, aqueous solutions, blood, plasma) without the need of organic solvents or surfactant.
- iii) to display high selectivity and not to interact with other endogenous bio-thiols (*i.e.*, glutathione, cysteine ...) or other ions present in blood or tissues under investigation.
- iv) to exhibit very low or no cytotoxicity to be promising for further development (bio-compatible & bio-degradable).
- v) to emit in the near-infrared preferably at 700–900 nm as this permits greater tissue penetration, causes less cellular photo-damage or phototoxicity and minimizes the interference from background auto-fluorescence. The emission is preferably accompanied by large Stokes shift, as small Stokes shifts may lead to measurement errors such as auto-quenching and/or excitation back-scattering [39]
- vi) to be functionalized to target certain subcellular organelles (mitochondria, lysosome, nucleus, endoplasmic reticulum, ...), certain cells (hepatocytes, ...), tissues, or organs.

Based on H₂S main chemical properties *i.e.*, nucleophilicity, reducibility, and metal precipitation capability, researchers have developed a large number of fluorescent molecules which can be classified according to their H₂S-reactive sites or chemical reaction-based sensors as detailed in the next sections and summarized in Table 1 highlighting the main advantages, disadvantages, and applications of each probe.

Reduction-based fluorescence compounds:

These compounds contain an easily reducible group such as azide [40], nitro [41], or hydroxylamine [42], which act generally as fluorescence quenchers. These quenchers are linked to a fluorophore nucleus such as coumarin [43], rhodamine [44], chromone [45], cyanine [41], benzopyran derivative [46], dansyl [47], naphthalimide either as a molecular sensor [42,48] or incorporated in a nanosensor [49]. The reaction proceeds *via* their reduction to their corresponding amines under physiological conditions.

H₂S-activated fluorescent sensors are mainly based on the difference of emission wavelength and quantum yield before and after reaction with free sulfide or measuring differential fluorescence response at two different wavelengths. Based on the fluorescence signal(s) and post-measurement data analysis, such category can be further subdivided into:

- i) **Fluorescence Turn-on:** Principle entails measuring the increase in fluorescence emission. Since the first reported probe based on the reduction of non-fluorescent azides to fluorescent amines, compound **F1**, many azide-containing probes were developed, Table 1. Although compound **F1** exhibits fluorescence emission in the near infra-red region

(700 nm) and was used for monitoring H₂S in HEK293 T cells it displays lower selectivity with relatively long response time (30 min) [40]. Another compound **F4** was developed to target lysosome, containing a spirolactam moiety which opens in lysosomal acidic microenvironments, while its azide group is reduced by H₂S giving a fluorescent derivative, albeit it exhibits small Stokes shift [44]. Whereas compound **F5**, was synthesized to target the mitochondria and for the first time to target the nucleus, however, it suffers from photosensitivity alongside a slow response (60 min) [43]. A sensitive fluorogenic nanoprobe containing azide having a good sensitivity (LOD = 18 nM) was introduced to determine H₂S *in vitro* (living cells and mice serum) and the differentiation between sera of diabetic and non-diabetic mice [50]. Recently, a hepatocyte-targeting sensor, **F7** containing galactosyl moiety was developed due to the specific recognition of ASGPR over-expressed in hepatocytes by galactose group. It displays fast response (\approx 1 min) with good selectivity and sensitivity (LOD = 126 nM) [51].

- ii) **Fluorescence Turn -Off:** It is based on measuring the decrease in fluorescence emission. Many sensors were developed exhibiting “turn-off” fluorescence response, Table 1. for example compound **F9** contains an azide group linked to rhodamine derivative as a fluorophore [52]. This compound was used for quantifying H₂S in human embryonic kidney 293 T cells and could target mitochondria but it suffers from relatively long response time (40 min). Another boron-dipyrromethene (BODIPY) derivative was developed to detect H₂S in normal human oral fibroblast cells with good sensitivity 170 nM but still suffers from long response time (20 min) in a medium containing 33% methanol [53]. Organic solvents have certain limitations which may hamper further development for *in vivo* applications. For example, DMSO exhibits hemolytic activity and a significant effect on cellular membrane permeability. Moreover, it induces apoptosis of the vascular endothelial cells [54], whereas ethanol mediates for red blood cell hemolysis [55].
- iii) **Ratiometric analysis:** It measures the intensity ratio changes at two emission wavelengths which generally offers more accurate results than turn-on and turn-off because it does not generate false positive/negative signals nor it is affected by analyte-independent interfering factors, such as the excitation source fluctuation, sample matrix background light scattering and autofluorescence, the microenvironment around the probe, and variation of the local concentration of the probe [33]. The first ratiometric fluorescent probe is an azido-heptamethine cyanine dye (compound **F2**) that exhibits emission in NIR (greater than 700 nm) with good sensitivity (LOD = 80 nM) and was found able to detect changes in H₂S levels in macrophage RAW264.7 cells, though to display long response time (20 min) as its only caveat [49,56].

Recently, a portable H₂S analyzer was proposed as a simple determination of H₂S in both aqueous solution and plasma using a fluorescent probe. The developed method was applied and validated for the quantification of H₂S in plasma of cardiovascular patients [15]. The developed fluorescent sensor relied on the use of an azide derivative (an H₂S reduction-based mechanism) [47]. However, this probe was not examined against the most abundant biothiols as GSH which represents a limitation for its biological application. Moreover, the derivatizing medium contains tween 20 which is known for its hemolytic activity [57] and to account for its validation using plasma and not on whole blood. Another recent study developed a microfluidic method for the measure-

ment of sulfide in blood plasma that relied on using the same fluorescent sensor dansyl azide, which confirmed the plasma matrix interference. Though a dilution step 3.3-fold dilution is required to reduce plasma interaction with exogenous sulfide [58].

Electrophile-based probes

These chemicals encompass at least one or two electrophilic centers to be attacked *via* nucleophilic addition/substitution reac-

Table 1
Representative examples of certain fluorescent sensors for H₂S determination with the advantages and disadvantages of each probe.








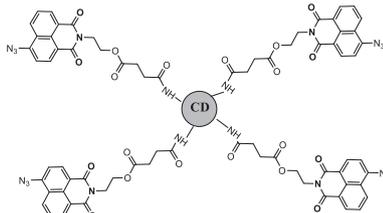
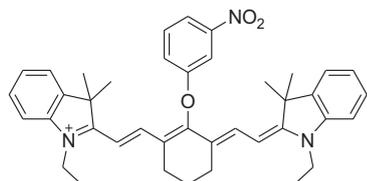


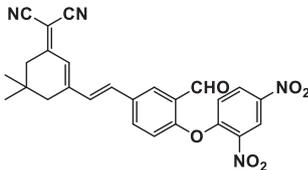


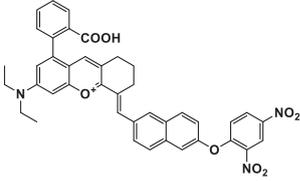


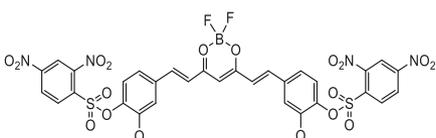

N°	Sensor	Properties & Applications	Ref.
A) Reduction-based fluorescence compounds			
F1		Adv.: emission in the NIR (700 nm) Disadv.: relative long response (sulfide-sensor reaction) time (30 min), detection medium contains DMF, unsatisfactory selectivity (2- & 5-fold increased selectivity versus O ₂ & GSH/Cys, respectively) Application: living Cells (HEK293T cells)	[40]
F2		Adv.: emission in the NIR (> 700 nm), Stokes shift = 90 nm; low LOD (80 nM); detection medium: 100% aqueous Disadv.: relative high response time (20 min) Application: living Cells (RAW264.7) Macrophage cells	[56]
F3		Adv.: near infrared emission (670 nm) with large Stokes shift (150 nm) Disadv.: detection medium contains high DMSO concentration (50%), long response time (60 min), high LOD 3050 nM Application: bovine serum, living cells (HeLa & MCF-7), tissues (fresh rat liver cancer slice) & live mice (monitoring localized diffusion after a dorsal skin-pop injection)	[165]
F4		Adv.: targeting lysosome (morpholine moiety), Disadv.: medium contains 10% DMF, small Stokes shift (25 nm) λ _{ex/em} = 530/555 nm Application: exogenous & endogenous H ₂ S in lysosomes of living cells (HeLa)	[44]
F5		Adv.: 35-fold fluorescence enhancement, mitochondria-targeted and 1st time target nucleus Disadv.: photosensitive, large response time (60 min), detection medium contains DMSO (2%), not specified LOD, small Stokes shift (45 nm) λ _{ex/em} = 405 – 450 nm Application: living cells (HeLa)	[43]
F6		Adv.: near infrared emission (710 nm), detection medium aqueous (PBS) Disadv.: long response time (40 min); small Stokes shift (60 nm), Application: mitochondria / human embryonic kidney (HEK) 293 T & HeLa cells	[52]
F7		Adv.: good hepatocyte-targeting, excellent water solubility, low cytotoxicity, fast response (within 1 min), high selectivity, good sensitivity (LOD 126 nM) Application: hepatocyte-targeting	[51]
F8		Adv.: wide pH range (4–9), good sensitivity (LOD = 10 nM) Disadv.: relative long response time (15 min), the medium contains ethanol (25%), UV excitation (340 nm) Application: <i>in vitro</i> exogenous H ₂ S in HeLa (human cervical cancer cell) and L929 (murine aneuploid fibrosarcoma cell)	[49]
F9		Adv.: both excitation and emission in the NIR (755/809 nm), aqueous medium, large linear range 0 – 350 μM, wide pH range 4.2 – 8.2 Disadv.: relative small Stokes shift (54 nm), moderate quantum yield (0.11); 12.7 fold fluorescence enhancement, the long response time (60 min); biothiols as GSH & Cys interfere with H ₂ S determination Application: living cells (RAW264.7)	[41]
F10		Adv.: 13-fold fluorescence enhancement, satisfactory sensitivity (LOD 500 nM), Quantum yield 0.12 λ _{ex/em} = 435 / 544 nm Disadv.: very long response time (120 min); Interference with sod. ascorbate Application: living cells (Astrocyte cells)	[42]

Table 1 (continued)

N°	Sensor	Properties & Applications	Ref.
B) Electrophile-based probes (containing 2,4-dinitrophenyl moiety)			
F11		Adv.: very fast response time (4 sec.), NIR emission (680 nm), 115 fold fluorescence enhancement, linearity range (1–10 μ M), good sensitivity (LOD = 11 nM), satisfactory Stokes shift (90 nm $\lambda_{ex/em}$ = 590/680 nm), aqueous detection medium (PBS), low cytotoxicity against different cellular lines Application: lysosome-targeting/cell (HeLa) and mice (monitoring localized diffusion after intraperitoneal injection)	[59]
F12		Adv.: relative rapid response time (10 min), NIR emission (663 nm), very large Stokes shift (244 nm), 105-fold fluorescence enhancement, good sensitivity (LOD = 42 nM), good selectivity, linear range 0 – 50 μ M, wide pH range (6 – 10), good quantum yield = 0.22 Disadv.: detection medium contains DMSO (30%), not for acidic pH Application: exo & endogenous H ₂ S <i>in vitro</i> (HeLa cells)	[166]
F13		Adv.: rapid response time (4 min), 32-fold fluorescence enhancement, good quantum yield (0.45); good sensitivity (LOD = 150 nM) linear range 0 – 100 μ M, pH range (5 – 10), aqueous detection medium (4-(2-hydroxyethyl)-1-piperazineethanesulfonic acid buffer) Disadv.: GSH reacts with the probe but at a lesser extent (slower rate) than sulfide Application: target endoplasmic reticulum, endogenous & exogenous H ₂ S imaging in living cells	[167]
F14		Adv.: NIR fluorescent probe, linear range (12–38 μ M), large Stokes shift (97 nm, $\lambda_{ex/em}$ = 543 nm / 640 nm) Disadv.: high LOD 3090 nM, very long response time (170 min) & time-dependent fluorescence increase, certain anions as dihydrogen phosphate respond to the probe, The sensor was not tested against biological thiols (GSH, Cys, ...) to evaluate their possible interferences. Application: detect molecular H ₂ S in the gaseous state, H ₂ S in real water, red wine and living cells (MCF-7 (human breast carcinoma) cells)	[94]
F15		Adv.: rapid response (3 min); near-infrared fluorescent probe, 11-fold fluorescence enhancement; large Stokes shift (107 nm, $\lambda_{ex/em}$ = 557 / 664 nm), quantum yield (0.11), linear range (0 to 30 μ M) with LOD (68.2 nM), high selectivity Disadv.: medium contains DMSO & disodium phosphate dodecahydrate Application: living cells (Hela cells) / mitochondria-targeting	[168]
F16		Adv.: NIR emission, 169-fold fluorescence enhancement, LOD = 121 nM, pH range 5 – 8.5, good selectivity Disadv.: time – dependent fluorescence increase (linearly up-to 180 min); small Stokes shift (49 nm, $\lambda_{ex/em}$ = 590/639 nm), detection medium contains DMSO (10%) Application: HeLa cells / lysosome-targeting	[67]
F17		Adv.: rapid response time (less than 1 min), fluorescence enhancement 130-fold, very large Stokes shift (221 nm, $\lambda_{ex/em}$ = 445/666 nm), good sensitivity (LOD = 6 nM) Disadv.: detection medium contains DMSO (20%) Application: HeLa cells/mice	[63]
F18		Adv.: good sensitivity (LOD = 50 nM), wide linear range 0 – 275 μ M, Stable over wide pH range, good selectivity, large Stokes shift (140 nm, $\lambda_{ex/em}$ = 415 / 555 nm) Disadv.: slow response time (40 min), 6-fold fluorescence enhancement, detection medium contains DMSO (2.5%) Application: spiked rat urine samples, exogenous & artificially generated endogenous H ₂ S in living cells (Hela) & <i>in vivo</i> living <i>Caenorhabditis elegans</i> (nematodes)	[64]
F19		Adv.: relative rapid response time (2 min), NIR emission (652 nm), 35-fold FL enhancement, good sensitivity (LOD = 10 nM), good selectivity, large Stokes shift (128 nm, $\lambda_{ex/em}$ = 512 / 652 nm), Stable over 6 – 10 pH, Linear range 0 – 30 μ M Disadv.: weak quantum yield (0.067), detection medium contains high organic solvent DMF (50%), not for acidic pH Application: imaging exogenous H ₂ S in HeLa cells & artificially generated endogenous H ₂ S in RAW264.7 cells, <i>in vivo</i> (Kunming mice)	[65]

(continued on next page)

Table 1 (continued)

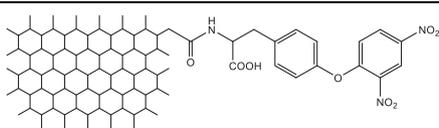
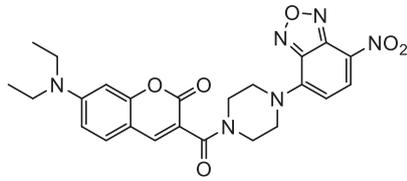

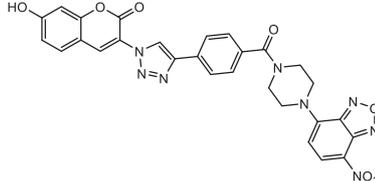






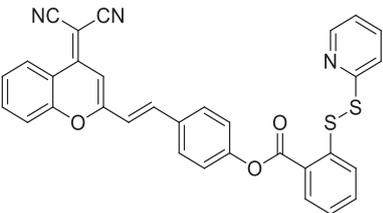
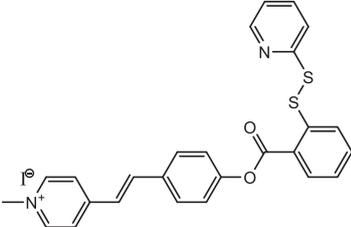
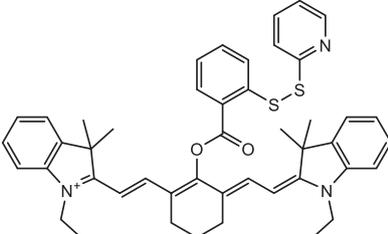



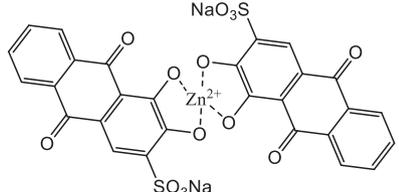
N°	Sensor	Properties & Applications	Ref.
F20		Adv.: relative rapid response time (10 min), good selectivity, high sensitivity (LOD = 0.89 nM), wide linear range 2 nM – 1500 nM, Low cytotoxicity Disadv.: small Stokes shift (54 nm, $\lambda_{ex/em}$ = 480/534 nm) Application: living cells (MCF7)	[62]
B) Electrophile-based probes (containing NBD (7-nitro-1,2,3-benzoxadiazole))			
F21		Adv.: 45-fold fluorescence enhancement, satisfactory Stokes shift (75 nm, $\lambda_{ex/em}$ = 405/480 nm), 1st fluorescent probe based on thiolysis of NBD amine Disadv.: relative slow response time (30 min), low sensitivity (LOD = 9000 nM), Application: living cells (HEK293 & HeLa cells)	[72]
F22		Adv.: mitochondria-targeting, 68-fold fluorescence enhancement, low cytotoxicity, biocompatible, good selectivity. Disadv.: slow response time (40 min), moderate sensitivity (LOD = 2460 nM), small Stokes shift (53 nm $\lambda_{ex/em}$ = 394 / 532 nm) and detection medium contains CH ₃ CN (10%) Application: HeLa cells (Mitochondria).	[71]
F23		Adv.: 45-fold fluorescence enhancement, good sensitivity (LOD = 56 nM), good selectivity, good Stokes shift (92 nm, $\lambda_{ex/em}$ = 394/486 nm) Disadv.: response time (20 min), narrow pH range (7.4–8.5), medium contains DMSO (10%) Application: H ₂ O ₂ -induced H ₂ S release in Yeast cells	[66]
F24		Adv.: rapid response (~3 min), 4.5-fold fluorescence enhancement, Quantum yield = 0.36, linear range (0–30 μ M), satisfactory sensitivity (LOD = 580 nM), pH rang (6–8.5) Disadv.: sulfites ions react but at a lesser extent than sulfides, small Stokes shift (22 nm, $\lambda_{ex/em}$ = 567/589 nm) Application: H ₂ O ₂ -induced H ₂ S biogenesis in living cells.	[68]
F25		Adv.: rapid response time (5 min), 17-fold fluorescence enhancement, LOD = 9.6 nM, pH range 5 – 8, good selectivity Disadv.: detection medium contains DMSO (10%); small Stokes shift (49 nm, $\lambda_{ex/em}$ = 590 / 639 nm) Application: HeLa cells / Lysosome-targeting	[67]
B) Electrophile-based probes (containing aromatic carbonyl with adjacent α,β-unsaturated carbonyl compound)			
F26		Adv.: relative rapid response time (20 min), 13-fold fluorescence enhancement, better quantum yield = 0.208 Disadv.: small red shift (Stokes shift = 45 nm, $\lambda_{ex/em}$ = 465 / 510 nm) with low sensitivity (LOD = 5000 nM), detection medium contains DMSO (1%) & time-dependent (0 – 60 min) fluorescent increase Application: <i>in vitro</i> HeLa cells	[73]
F27		Adv.: satisfactory Stokes shift 55 nm, pH range (5–8), Disadv.: energetic excitation (308 nm), Medium contains DMSO (10%), limited sensitivity (high LOD 1700 nM), Application: living cells (Vero)	[74]

Table 1 (continued)

N°	Sensor	Properties & Applications	Ref.
F28		Adv.: good sensitivity (LOD = 160 nM), linear range (0 – 10 μM), wide pH range (3 – 9), large Stokes shift (108 nm, $\lambda_{ex/em}$ = 445 – 577 nm) Disadv.: long response time (40 min), detection medium contains DMSO Application: HepG2 cells and Chlorella	[75]
B) Electrophile-based probes (containing (disulfide or selenenyl sulfide) benzoate ester)			
F29		Adv.: fluorescence enhancement 15-fold; good selectivity, good sensitivity LOD = 790 nM, large Stokes shift (108 nm, $\lambda_{ex/em}$ = 345/453 nm), linear range (0–300 μM) Disadv.: long response time (30 min); energetic excitation wavelength, detection medium contains CH ₃ CN (30%) and CTAB 1 mM Application: endogenous and exogenous H ₂ S in HeLa cells, Drosophila, melanogaster and C. elegans	[169]
F30		Adv.: NIR emission, good sensitivity LOD (1.1 nM), large Stokes shift (120 nm, $\lambda_{ex/em}$ = 560/680 nm) Disadv.: long response time (30 min), detection medium: containing 50% DMSO/PBS Application: living cells	[76]
F31		Adv.: 10-fold fluorescence enhancement, linear range: 2–14 μM; LOD 25.7 nM, pH range (7–10), Disadv.: relative long reaction time (15 min), biothiols as (L- Cys, Hcy, GSH) were tested at the same H ₂ S concentrations (50 μM) medium contains DMF (10%), Application: living cells (HeLa)	[170]
F32		Adv.: NIR emission, Quantum yield (0.19), 22-fold fluorescence enhancement, pH range 6–12, good sensitivity 36 nM, large Stokes shift (129 nm, $\lambda_{ex/em}$ = 510/639 nm) Disadv.: narrow linear range (1–6 μM), the medium contains DMF (10%), the long response time (60 min), biothiols as (L- Cys, L-methionine) reacts with the probe but at the lesser extent and they were tested at lower concentrations (50 μM vs 20 μM H ₂ S) Application: target mitochondria, <i>in vitro</i> (HeLa cell), <i>in vivo</i> (mice)	[80]
C) Probes induced metal-sulfide precipitation			
F33		Adv.: 100% aqueous medium, rapid response time (instantaneous), large Stokes shift (161 nm, $\lambda_{ex/em}$ = 256, 417 nm), good selectivity, no cytotoxicity (up to 100 μM, WST-1 cells) Disadv.: UV excitation range (energetic), relative low sensitivity (LOD = 3900 nm), pH range is not checked Application: living cells, HeLa cells treated with exogenous H ₂ S	[83]
F34		Adv.: 100% aqueous medium, rapid response time (1 min), satisfactory Stokes shift (55 nm, $\lambda_{ex/em}$ = 375, 430 nm), high quantum yield (0.65), good sensitivity (205 nM), Disadv.: biothiols as Cys react with the sensor but at a lesser extent than sulfide Application: living cells (HeLa), <i>in vivo</i> (Zebra fish)	[171]

(continued on next page)

Table 1 (continued)

N°	Sensor	Properties & Applications	Ref.
F35		Adv.: satisfactory sensitivity (LOD 250 nM), good aqueous solubility, the rapid response time (less than 1 min), satisfactory Stokes shift (66 nm, $\lambda_{ex/em}$: 480/546 nm) Disadv.: biothiols as Cys & GSH were tested at the same concentration (20 μ M) as NaHS (not relevant to physiological concentration ratios). Application: living cells, HeLa cells treated with exogenous H ₂ S	[172]
F36		Adv.: NIR emission, fast response time (30 sec), good sensitivity (LOD 92 nM), good aqueous solubility, large Stokes shift (95 nm, $\lambda_{ex/em}$: 530/625 nm) Disadv.: highly pH-dependent fluorescence, narrow pH range (7–8), the medium contains MeOH (75%). Application: human serum and bovine serum albumin, living cells, (C-6 cells) treated with exogenous H ₂ S	[82]

tion to yield a thio-derivative, followed by another intramolecular nucleophilic addition/substitution of H₂S to the probe. This results in one or two fluorescent compounds

- i) *2,4-dinitrophenyl-based probes:* The 2,4-dinitrophenyl moiety acts as a quencher of the fluorophore moiety via photo-induced electron transfer (PET). 2,4-Dinitrophenyl moiety can be linked to the fluorophore nucleus such as cyanine [59], xanthene [60], pyridinium derivative [46], pyrimidine derivative [61], functionalized graphene quantum dots [62] via an ether linkage, or a sulfonamide linkage to fluorophore as dicyanoisophorone [63], curcumin [64], coumarin [65].

The reaction with H₂S proceeds via nucleophilic addition of H₂S to the probe generating a thiol derivative which undergoes subsequent intramolecular nucleophilic substitution (thiolysis) and cleavage of the linkage (i.e., ether, sulfonamide, and ester) liberating the fluorophore (parent fluorescent dye).

As illustrated in Table 1, this family of compounds exhibits various advantages according to the fluorophore derivatives being employed leading to emission in NIR as compounds **F11**, **12**, **15**, **17**, **19** with very large Stokes shift (244 nm) exemplified in compound **F12**. Certain intracellular organelles could be targeted as lysosome (**F17**), endoplasmic reticulum (**F13**), or mitochondria (**F15**). A sensitive fluorescent sensor, **F23** (LOD = 11 nM) contains an ether-linkage and cyanine derivative (fluorophore) was developed to react instantaneously with H₂S (4 sec) exhibiting 115-fold fluorescence enhancement (Turn-on). It offers a water-soluble sensor that has been used in cellular imaging (HeLa and HepG2), lysosomes, and *in vivo* in mice [59]. The fluorescence enhancement is generally reflecting the increase in the fluorescence intensity in the presence of sulfide compared to that of the probe alone under the give reaction conditions (Time, temperature, pH,).

The first developed sensor containing sulphonamide linkage was that of compound **F17**, as a new selective reaction site for H₂S, between the 2,4-dinitrophenyl moiety (quencher) and dicyanoisophorone (fluorophore) exhibited high sensitivity (LOD = 6 nM), rapid response (less than 1 min), large Stokes shift (221 nm) and has been used in cellular imaging and *in vivo* in mice [63].

Graphene quantum dots-based sensor, **F20** offers the highest sensitivity (LOD 0.89 nM) of this family with wide linear range (2 – 1500 nM) and used for H₂S detection in MCF7 but it displays excitation /emission out of the NIR with relative short Stokes shift and relative long response time (10 min).

- ii) *NBD (7-nitro-1,2,3- benzoxadiazole)-based probes:* The 7-nitro-1,2,3- benzoxadiazole acts as a quencher of the fluorophore. The fluorophore moiety can belong to coumarins [66], rhodamine B amines [68,69], Tetrahydro [5] helicene [70], naphthalimide [71] all linked to NBD via different linkers as ether or thioether bond. As the reaction proceeds, under physiological pH via the attack of the nucleophilic sulfhydryl group to the probe generating a thiol derivative which undergoes subsequent intramolecular nucleophilic substitution (thiolysis), liberating the non-fluorescent thio-NBD derivative and the fluorophore. Therefore, all the NBD-based H₂S sensors exhibit turn off-on fluorescence response.

As illustrated in Table 1, compound **F21** was the first synthesized NBD-based H₂S sensor used for its detection *in vitro* in living cells (HEK293 and HeLa cells) [72], after which many NBD-based H₂S sensors were developed to improve sensor features such as sensitivity level [66], or to target certain organelles as lysosomes using compound **F25** [67] or mitochondria using compound **F22** [71]).

- iii) *Aromatic carbonyl with adjacent α,β -unsaturated carbonyl-based probes (Michael acceptor):*

The reaction in these probes proceeds via two mechanisms. First, it involves a double nucleophilic addition in which H₂S attacks the aromatic carbonyl group generating a thiol derivative which undergoes subsequent Michael addition to yield the acrylate ester (α,β -unsaturated carbonyl compound (Michael acceptor) leading to cyclic fluorescent thio-derivative [73,74]. Second, it functions via a double nucleophilic attack, initially through HS⁻ nucleophilic substitution generating a thiol derivative that undergoes subsequent intramolecular nucleophilic addition that leads to cyclic non-fluorescent compound (Turn-off) carbazole derivative [75]. As illustrated in Table 1, compounds **F26-28** were used for *in vitro* H₂S cellular imaging (HeLa, Vero, and HepG2 cells), albeit they use relatively energetic excitation wavelengths (308–465 nm) with subsequent increased risk of cellular photo-damage or phototoxicity. Furthermore, these sensors displayed a relatively long response time (20–40 min) and moreover failing to attain high sensitivity (160 nM – 5000 nM).

- iv) *Probes containing (disulfide or selenenyl sulfide) benzoate ester-linked to a fluorophore*

The reaction proceeds via two consecutive nucleophilic substitutions initially through HS⁻ nucleophilic substitution generating

a thiol derivative which undergoes subsequent intramolecular nucleophilic substitution and cleavage leading to a fluorophore and cyclic non-fluorescent thio-compound [76,77]. The first disulfide-based sensors were developed [78] with the drawback of overconsumption of biothiols and thus high probe loading was needed. Certain biothiols (RSH) as glutathione, L-cysteine, and Homocysteine could undergo the first substitution step consuming part of the sensor but could not proceed beyond. As these biothiols do not possess more than one replaceable proton, which prevents the achievement of the second nucleophilic substitution step and consequently blocking the cyclization and the fluorophore liberation. It is worth noting that glutathione (GSH) represents the most abundant cellular biothiols (1–10 mM) [79]. Though GSH should be evaluated its potential interference at least (1 mM) 10 times H_2S biological concentrations which were in the nano-micromolar range [38]. Many sensors were tested even at a higher GSH/ H_2S concentration ratio (20x) as in the case of compounds **F11**, **F15**, **F19**, and **F26**. However, the selectivity is questionable for certain sensors which evaluated at lower GSH/ H_2S concentration ratio or even at the same sulfide concentration as in the case of compounds **F31** and **F32**. As shown in Table 1, compounds belonging to this family of sensors exhibit emission in NIR with very large Stokes shift (120 and 129 nm) and display good sensitivity (LOD = 1.1 and 36 nM) as exemplified in compounds **F30** and **F32**, respectively. Certain intracellular organelles could be targeted as mitochondria to detect H_2S as compound **F53**. However, biothiols still show slight interference [80], which may be attributed to the contribution of other nucleophilic centers in these interfering molecules leading to cyclization and liberation of the fluorophore.

As the pK_a of H_2S (6.9) is lower than that of most abundant cellular biothiols such as GSH (9.2), Hcys (8.9), Cys (8.3), indicating that H_2S has a stronger nucleophilicity than other biothiols under physiological conditions pH (7.4). However, it is still somewhat difficult to distinguish GSH/Hcys/Cys from H_2S simply via nucleophilic reaction-based strategies and affecting quantification results due to such interference

Probes induced metal-sulfide precipitation

- These probes (metal–ligand compounds) contain a fluorescent moiety, chelating agent, and transition metal cations as Cu^{2+} , Zn^{2+} , Hg^{2+} , with to act as a quencher (Turn-off) [29]. The fluorescence turn-on, is driven by precipitation of the metal sulfide (CuS , ZnS , $K_{sp} = 6.4 \times 10^{-36}$, 1.6×10^{-24}) [81,82].

As shown in Table 1, a copper-based H_2S fluorescent sensor compound **F33** was synthesized, containing anthracene derivative (fluorophore) attached to azamacrocyclic ring (ligand) as a Cu^{2+} -chelator to form a stable metal complex [83]. The paramagnetic Cu^{2+} center serves to quench the fluorophore's fluorescence upon H_2S binding to Cu^{2+} , which is then extracted from the azamacrocyclic ring resulting in enhanced fluorescence. The probe compound **F33** exhibited a fast response with good selectivity for *in vitro* fluorescence imaging of cellular H_2S in HeLa cells treated with exogenous H_2S . A zinc-based sensor F36, exhibits emission in NIR with fast response displaying good sensitivity (LOD = 92 nM). It is used for H_2S monitoring and quantification in living cells (C-6) and human and bovine sera. However, this sensor is highly pH-dependent with a narrow pH range (7–8).

Nanotechnology has been increasingly implemented in the development of nanosensor based on metal-sulfide precipitation. A turn-on fluorescent probe based on Cu-porphyrin coordination complex combined with gold nanoparticles was developed and applied for H_2S *in vitro* measurement in two carcinoma cell lines (A549 and H1299 cells). Although this nanosensor exhibited NIR emission (650 nm) and good sensitivity (LOD = 17 nM) and selectivity against most interfering ions and biothiols, certain biothiol as

Cys showed cross-reaction but at a less extent than sulfide, besides from its relatively slow response time (20 min) than H_2S itself [84]. Another fluorescent nanosensor based on carbon quantum dots/silver nanoparticles (CQDs-AgNPs) exhibits one of the most sensitive methods with an LOD = 0.4 nM. This sensor was used for the *in vivo* monitoring of H_2S basal level (3.08 μM) and cerebral H_2S level in rat brain during the calm/ischemia states, whereas the linear detection level ranged from 0.001 to 1.9 μM [85]. An easily synthesized fluorescent gold-based nanoclusters were recently reported for H_2S detection in living cells (SMMC-7721). This sensor offers several advantages as good aqueous solubility, biocompatibility, high selectivity, wide linear range (27 pM – 850 μM), and with an outstanding LOD (24 pM) [86].

However, Cu (II) containing probes, turn-on *via* CuS precipitation may be interfered by other biological reducing species such as NO, HNO, which occur *via* metal displacement by His and Cys, reduction of Cu(II) to Cu(I), or hampered by other competitive pathways to remove the metal quencher [87]. Though, a more selective or even specific chemical reaction may be needed to overcome the interfering endogenous similar chemical species or other competitive pathways. Taking into consideration the chemical properties of H_2S and the expected sulfide form. [48]



According to pK_a of H_2S , temperature, and medium pH, H_2S equilibrates with its two anions HS^- and S^{2-} where the three forms exist at different proportions and Eq.1 represents the real dynamics of H_2S in solution [13]. However, and according to Le Châtelier's principle, this equilibrium will continuously shift to either side. For example, it has been reported that half of H_2S escapes from solution in five minutes in cell culture wells and 0.5 min in the Langendorff heart apparatus [88]. In subcellular organelles the relative free sulfide proportions, from 90% of HS^- in mitochondria (pH = 8) to more than 90% of H_2S in lysosomes (pH = 4.7) [89]. Therefore, according to the reaction mechanism and the effective working pH, H_2S -probe is destined selectively to one form of the three H_2S species. Considering that certain H_2S -sensors were selectively reacted with the unionized form (H_2S) in a reduction-based reaction (azide, nitro, hydroxylamine,...) [23,14]. Whereas electrophile-based probes based on the double nucleophilic attack were destined to the most abundant physiological sulfide ion (HS^-) [90], while metal displacement-based reactions (Cu^{2+} , Zn^{2+} , Hg^{2+} ,...) are destined selectively to the dianionic counterpart (S^{2-}) [91]. It is worth mentioning that most of the analytical methods used mainly Na_2S , the least abundant physiological sulfide ion (S^{2-}), in different pH media to carry out either *in vitro* or *in vivo* investigations [15,47,92–94].

Colorimetric based assays

Colorimetric methods are assays that are based on spectral changes upon the interaction of chromogen with a particular analyte. Such changes could be monitored using simple instrumentation i.e. spectrophotometers. Colorimetric methods have particularly been employed for H_2S determination (Table 2) due to ease of use, fast reaction time and characteristic absorption bands to overcome interference especially in the case of biological samples [95].

Classical colorimetric methods

One of the earliest and most common methods used for H_2S measurements is the methylene blue reaction of sulfide with *N,N*-dimethyl-*p*-phenylenediamine, in the presence of ferric chloride to yield a blue color that could be measured spectrophotometri-

Table 2Representative examples of certain colorimetric sensors for H₂S detection with the advantages and disadvantages of each probe.

Probe	Principle	Properties & applications	Ref.
<i>N,N</i> -dimethyl- <i>p</i> -phenylenediamine	Spectrophotometric detection of the developed methylene blue dye at 670 nm after trapping of H ₂ S with Zn ²⁺ .	Adv.: a simple protocol Disadv.: lack of selectivity for H ₂ S, not suitable for <i>in vivo</i> H ₂ S determination Application: <i>in vitro</i> samples	[97]
NBD-Cl	Thiolysis of NBD-Cl upon reaction with H ₂ S to form nitrobenzofurazan thiol (Pluth red) <i>via</i> a nucleophilic aromatic substitution reaction	Adv.: fast reaction time, used for both biological and environmental applications, selective. Application: fetal bovine serum	[98]
Azine based sensor	Deprotonation of the sensor –OH	Adv.: selective, fast response time (less than a minute) Disadv.: low sensitivity (LOD 18.2 μM) Application: human and mouse sera	[95]
1-(2-Pyridylazo)-2-naphthol-Cu ²⁺	Displacing Cu ²⁺ from its complex through a metal S ²⁻ formation	Adv.: enhanced sensitivity with LOD 2.5 μM Disadv.: No biological studies or real sample analysis Application: aqueous H ₂ S	[99]
Boron-dipyrromethene-Cu ²⁺		Adv.: detection of gaseous H ₂ S with LOD 16 ppb Application: gaseous H ₂ S Adv.: good selectivity for the H ₂ S, LOD (0.167 μM), fast reaction time Disadv.: no biological studies or real sample analysis Application: aqueous H ₂ S	[100]
Ag NPs /Nafion polymer	The reaction of Ag NPs with S ²⁻ to form Ag ₂ S with strong absorbance band at 310 nm	Adv.: simple microplate-based colorimetric assay Application: mouse liver homogenate	[101]
Ag NPs / Nafion/ PVP polymer		Adv.: wide linear dynamic range for H ₂ S (6.25 to 50 μM) with LOD 1 μM. Application: C6 glioma cells	[102]
Ag NPs in a layer-by-layer polyelectrolyte multilayer film	UV–vis measurement of the formed Ag ₂ S@Ag NPs at 430 nm.	Adv.: wide linear range 10 nM to 5 μM Disadv.: long reaction time (2 h for detection) Application: cellular endogenous H ₂ S gas.	[173]
Dopamine functionalized AgNPs	Decrease in the plasmon absorbance of AgNPs at 400 nm with a color change from bright yellow to dark brown observed by the naked eye.	Adv.: environmentally friendly, LOD 0.03 μM Disadv.: narrow linear range from 2 to 15 μM, Application: fetal bovine serum	[174]
PPF-AgNPs	Decrease in PPF-AgNPs absorption band at 400 nm upon reaction with H ₂ S	Adv.: good sensitivity and specificity, fast response time Application: various biological and environmental samples	[103]
Ag/Au core-shell nanoprism	Decrease in Ag/Au core-shell nanoprism absorption band at NIR region upon reaction with H ₂ S	Adv.: SPR peak is located in the NIR region Disadv.: long time (30 min) Application: serum	[104]
	Decrease in Ag/Au core-shell nanoprism absorption band at NIR region upon reaction with H ₂ S	Adv.: HS-SDME methodology, smartphone nanocolorimetry based detection set up, sensitive LOD 7 nM (UV – vis), and 65 nM(SCN). Application: egg and milk	[175]
Au-Ag core-shell	Quantification of RGB color variation of the Au-Ag core-shell resulting from the formation of Ag ₂ S on the particle surface.	Adv.: RGB colorimetric analysis, linear (50 nM to 100 μM) Disadv.: long time (20 min) Application: cell culture medium and the blood serum	[176]
Au/AgI dimeric nanoparticles	The color variation of the Au-Ag core-shell due to the formation of Ag ₂ S on the particle surface. AgI increases the probe selectivity	Adv.: linear (0 to 80 μM) with LOD of 0.5 μM (UV–vis spectrophotometer) Application: HepG2 cell	[105]
Glutathione capped AuNPs	AuNPs aggregation upon reaction with H ₂ S <i>via</i> ligand exchange reaction which results in a color change from red to purple/blue	Adv.: simple Disadv.: lower sensitivity level LOD (5 μM with a UV/vis spectrophotometer)	[106]
Fluorosurfactant functionalized gold nanorods (FSN-AuNRs)	FSN-AuNRs exhibits blue color changing to purple upon reaction with H ₂ S due to surface ligand substitution and aggregation of FSN-AuNRs	Adv.: capable of evaluating the activity of CBS Application: human and mouse serum samples	[107]
Au@TPt-NCs	Deactivation of the Au@TPt-NCs catalytic activity on (TMB / H ₂ O ₂ system) upon reaction with H ₂ S	Adv.: static headspace extraction was applied, with LOD 7.5 nM Application: newborn cattle serum	[108]
AuNRs	Deactivation of etching activity of (TMB /HRP) on AuNRs upon reaction with H ₂ S	Adv.: linear range 0.05–50 μM with a LOD of 19 nM Application: monitoring extracellular H ₂ S in rat brain	[177]

cally at 670 nm [96]. The method was later modified by trapping H₂S with zinc acetate to remove interference from other chromophores that might be present in the sample followed by acidification and subsequent formation of the dye [97]. However, several critical issues were observed when H₂S was determined in biological samples *viz.*, lack of selectivity and sensitivity, formed dimer and trimer of methylene blue that do not obey Beer's law, and finally, color formation is time-dependent which requires careful monitoring. On the other hand, Pluth's group reported a colorimetric method based on thiolysis of NBD-derived electrophiles; NBD-Cl reacts with H₂S *via* nucleophilic aromatic substitution reaction to form thioether followed by thiol formation of the unique color of NBD-SH (Pluth red) [98]. This method exhibited detection limit as low as 210 nM (buffer) and 380 nM (fetal bovine serum) and high selectivity for H₂S even in the presence of other

biologically-relevant nucleophiles such as glycine, serine, tyrosine, lysine, glutathione, and *N*-acetyl-cysteine. In another report for colorimetric H₂S determination, a new azine based sensor was developed for the selective determination of H₂S in physiological conditions. The method is based on deprotonation of one of the sensor –OH protons *via* reaction with H₂S resulting in a color change detected at 450 nm. The azine sensor exhibits a detection limit at 18.2 μM and has been applied successfully for H₂S quantitation in spiked mouse and human sera [95].

Displacement of copper complexes

Another colorimetric approach used for H₂S determination is through displacing a metal from its coordinated chromophore *via* metal sulfide formation resulting in a color change. This approach

has been widely employed for H₂S measurement due to its rapid response, reversibility, and robustness. Among the different metals-ligands displacement systems, copper complexes are the most widely employed sensors for H₂S analysis due to the very low solubility product of the formed CuS. Besides, the outstanding plasticity of the copper sphere facilitates Cu-complexes formation with a variety of chelating ligands [31].

Copper complex of 1-(2-pyridylazo)-2-naphthol was synthesized for the colorimetric sensing of aqueous sulfide with a pink to yellow color change upon displacement of Cu²⁺ from its complex [99]. Interestingly, the same probe has been developed for the quantification of gaseous H₂S via impregnating the probe with alkali on paper support [100]. The alkali will trap and convert the acidic H₂S gas to sulfide ion with a color change from pink to yellow. The probe could be coupled with a handheld colorimeter and a smartphone allowing quantification of H₂S gas or for its rapid detection with LOD of 16 ppb of gas. In another study, BODIPY and 8-aminoquinoline were incorporated for designing a colorimetric probe employed for H₂S detection. The probe forms 1:1 complex with Cu²⁺ in HEPES buffer with a decrease in the absorption band at 569 nm and an increase of a new band at 520 nm with a color change from pink to orange in rather fast reaction time. This method displays excellent selectivity towards sulfide over other competitive anions and thiols and with LOD of 0.167 μM in aqueous media [92].

Nanomaterials based colorimetric analysis

A recent colorimetric approach used for H₂S detection and quantification is based on the localized surface plasmon resonance (LSPR) optical traits of metal nanoparticles e.g. Ag NPs and Au NRs [19]. Compared to conventional colorimetric methods, plasmonic metal nanoparticles provide an exciting avenue for rapid and accurate determination of H₂S due to its higher photostability, lower photobleaching and intensity fluctuations, much higher scattering cross-section and extinction molar coefficients (REF). Exploiting the affinity of Ag⁺ to S²⁻, a wide range of colorimetric methods have been developed for H₂S determination. For example, Jarosz et al. [101] reported a microplate-based colorimetric assay using Nafion polymer doped with Ag⁺ ions for H₂S determination. Nafion polymer served as a template for Ag NPs synthesis where the formed Ag₂S NPs showed a strong UV absorbance at 310 nm. The same principle has been implemented in another study where polyvinylpyrrolidone (PVP) was utilized for Ag NPs construction being applied for measuring endogenous H₂S concentration in living C6 glioma cells [102]. Cross-linked polymer cages have been also employed as a potential medium for novel Ag NPs fabrication that was used in H₂S determination e.g. cross-linked polyhedral oligomeric silsesquioxane-formaldehyde polymer (PPF) [103]. PPF-AgNPs exhibit strong absorption at 400 nm which decreased quantitatively upon reaction with H₂S due to the formation of Ag₂S shell on the surface of PPF-AgNPs. The PPF-AgNPs exhibited excellent selectivity towards sulfide against other thiols and anionic species due to the specific Ag-S interaction within a linear range of 0.7–10 μM and a detection limit of 0.2 μM. Analysis of H₂S in various water and biological samples e.g. spring waste, urine, human serum and fetal calf serum using this novel probe have been demonstrated.

It is worth to note that some reports raised though doubt about the selectivity of silver nanoprobings for H₂S quantification, particularly in real samples with complicated matrices due to their susceptibility for oxidation in the presence of coordination agents such as hydrogen peroxide. Hence, several approaches were attempted to increase the selectivity of these nanoprobings via silver coating with a thin gold layer to form Ag/Au core-shell nanoprism that protect Ag from direct reaction with interfering species thus

increasing the latter's selectivity toward H₂S [104]. The defects in gold outer layer lateral walls allow reaction of only strong etching agents such as hydrogen sulfide with Ag nanoprisms and mitigate against interaction with other anions. This method exhibited a wide linear dynamic range from 0.1 and 10 μM with a detection limit of 54 nM and was applied for H₂S detection in serum. Interestingly, the same core-shell nanoprism has also been used in another study coupled with headspace single-drop microextraction (HS-SDME) to quantify H₂S. Smartphone nanocolorimetry (SNC) and UV – vis spectrophotometry were utilized to measure the change of Ag/Au core-shell SPR peak as a result of H₂S etching and both to demonstrate potential application for determining H₂S levels in real biological samples (egg and milk). In contrary to previous reports that employed Au as a protective shield for Ag NPs, Zeng et al [105] reported another strategy to increase Ag NPs selectivity based on engineering Au/AgI dimeric nanoparticles where the AgI acts as sensing agent and the Au acts as the signal-receptor core. Based on the fact that AgI exhibits the lowest solubility product among all silver halides, very few interfering compounds can react with stable AgI shell. These Au/AgI NPs have been immobilized into agarose gels to produce a solid form of “test strips” that has been applied successfully to determine H₂S gas concentrations released from Hep G2 cells during their cultivation.

Similar to AgNPs, AuNPs have been also widely used for H₂S determination due to the strong Au-S interaction. Such assays are based on the induction of AuNPs aggregation by inter-AuNPs crosslinking to result in color changes that can be easily observed by naked eyes (qualitative) or spectrophotometers (quantitative). For example, glutathione capped AuNPs have been used as an H₂S sensor via a ligand exchange reaction where sulfide will replace glutathione molecule on the AuNPs surface resulting in AuNPs aggregation and subsequent color change [106]. In a similar study, non-ionic fluorosurfactant capped with gold nanorods (FSN-AuNRs) has also been reported for the determination of H₂S [107]. In contrary to AuNPs, gold nanorods (AuNRs) possess two plasmon absorption bands responsible for their unique color change upon H₂S induced aggregation. This method exhibits high specificity towards sulfide over other anions and has been applied successfully for the determination of biological H₂S in both human and mouse serum as well as determining the activity of cystathionine β-synthase activity, the enzyme responsible for H₂S production. Interestingly, another AuNPs colorimetric strategy used for H₂S quantitative estimation is based on the H₂S-induced deactivation of (gold core)@(ultrathin platinum shell) nanocatalysts (Au@TPT-NCs) [108]. Upon target introduction, Au@TPT-NCs were deactivated to different degrees depending on H₂S levels, static headspace extraction was used with the Au@TPT-NCs as an effective sample pretreatment method for this system. This method displayed higher sensitivity for H₂S determination with a linear range of 10–100 nM and LOD of 7.5 nM. Besides, the method was applied for H₂S measurement in spiked real samples such as newborn cattle serum and although it is expedited route for the sensitive determination of biological H₂S *in vitro* samples, it has not been validated yet *in vivo*.

Phosphorescence analysis

Unlike fluorescence, phosphorescence is characterized by much longer emission lifetime which demonstrates its superiority in the bioimaging field [109]. Besides, the slow process of light re-emission entails the elimination of autofluorescence short-lived interference and improves S/N ratios. Among different phosphorescence probes for H₂S determination, transition metal complexes are known for their simple synthesis procedures and easy tuning of photophysical properties [110]. Novel iridium (III)-based luminescent turn on-off-on probe has been developed for the *in vitro*

and *in vivo* determination of sulfide ion [111]. This method is based on quenching of iridium (III) probe by Fe^{3+} , followed by restoring its luminescence upon the addition of sulfide. The probe exhibited a linear range from 0.01 to 1.5 mM, with LOD of 2.9 μM , and was successfully applied for sulfide imaging in living cells. In another report, an H_2S -associated phosphorescence turn-on probe was developed based on the *in situ* capturing of sulfide by Zn^{2+} and Mn^{2+} to form Mn-doped ZnS quantum dots [112]. These dots emit orange phosphorescence allowing elimination of autofluorescence interference from biological matrix and was thus employed for H_2S quantification in fetal calf serum with LOD of 0.2 μM .

Chemiluminescent analysis

Unlike other analytical techniques, chemiluminescence (CL) methods offer higher sensitivity and the wide dynamic range since the CL signal can be generated in the absence of any light sources which eliminates any background signal and improves the signal to noise for *in vivo* studies. Hence, they have been widely applied for the detection of disease biomarkers [113,114], including H_2S .

Among different CL systems, the reaction between luminol and hydrogen peroxide in the presence of horseradish peroxidase (HRP) as a catalyst is widely applied due to its simplicity and enhanced CL signal intensity. This triple system has been applied recently for H_2S determination in which H_2S deactivates HRP resulting in CL quenching of the system in a quantitative manner [115]. The method exhibits a linear dynamic range of 0.78–40 μM with a detection limit of 0.30 μM and has been applied successfully for H_2S determination in rat brain microdialysis. Another method used the irreversible reaction of H_2S with two masked azide-luminol scaffolds has been reported [116]. H_2S mediates the reduction of the azide moiety liberating luminol or isoluminol with enhanced CL intensity in the presence of H_2O_2 / HRP. The isoluminol based probe displays excellent selectivity for H_2S over a wide range of other biologically relevant reactive sulfur species, including thiols. Hence, it has been applied to measure the enzymatically produced H_2S effectively.

Electrochemiluminescence (ECL) is another luminescent process where an electrochemical reaction is employed to generate excited luminophore on an electrode surface via electron-transfer reactions [117]. ECL systems have been widely applied in H_2S detection due to their simplified optical setup, superior sensitivity, and low background signal level. For example, a cyclometallic iridium(III) complex has been synthesized as luminophore with high ECL intensity during cyclic voltammetry that quenches upon reacting with H_2S [118]. ECL signal of the system decreased linearly upon reacting with H_2S over a concentration range 40–140 μM with an estimated LOD of 11 nM. Another sensitive ECL was developed based on quenching ECL signal of the activated CdS nanocrystals film upon reaction with H_2S on a glass carbon electrode, in presence of other co-reactants such as H_2O_2 and citric acid, via bonding of sulfide to excess Cd^{2+} ions on the nanocrystals surface [119]. The method showed a wide linear range spanning from 5 nM to 20 μM and has been successfully applied for the determination of H_2S in calf serum. Furthermore, NBD-amine, a sensitive compound to H_2S , has been integrated with $\text{Ru}(\text{bpy})_3^{3+}$ -doped silica nanoprobe for sulfide quantification [120]. Nafion was used to immobilize $\text{Ru}(\text{bpy})_3^{3+}$ -doped silica on the surface of a glassy carbon electrode. The methods showed a linear range from 0.1 to 1×10^{-4} nM, LOD 1.7×10^{-6} nM and applied successfully to spiked human serum.

Cataluminescence (CTL) is another type of chemiluminescence in which the catalytic oxidation of analytes occurs on the surface of a solid material [121]. Among different types of CTL, metal-based catalysts represent the main type that exhibits high sensitivity for H_2S determination namely mesoporous SnO_2 [122], $\alpha\text{-Fe}_2\text{O}_3$

[123,124], microsphere In_2O_3 [125] and several alkaline-earth metal salts viz., CaCO_3 , SrCO_3 and BaCO_3 [126]. Also, metal-organic frameworks are also used for H_2S determination due to their large surface area, good thermal stability, and metal catalytic sites. ZIF-8 and $\text{Zn}_3(\text{BTC})_2 \cdot 12 \text{H}_2\text{O}$ are two examples of metal-organic frameworks whose LODs are 3.0 and 4.4 ppm for H_2S analysis, respectively [127]. Nevertheless, metal-based catalysts suffer from high cost, environmental pollution by heavy metals, and poor long-term stability. Albeit, these limitations can be overcome using metal-free catalysts such as nanocarbon catalysts which are stable on the long-terms, environmentally friendly, cost-effective, and highly selective. Silicon carbide (SiC) is a promising metal-free carbon material with distinct catalytic potential that has been enhanced by controlling its morphology through ion doping with fluorine [128]. SiC CTL signals display a linear relationship for H_2S quantitation in the range of 6.1–30.4 ppm with LOD 3.0 ppm.

Chromatographic methods

Although chromatographic methods for H_2S analysis could not be applied for real-time monitoring, they offer higher selectivity and specificity compared to direct spectrophotometric or fluorescence measurements. Separation technique as gas and liquid chromatography coupled to different sensitive detectors are considered as the mainstays for analysis of biological samples [38]. Chromatographic techniques are applied for H_2S detection in a wide range of biological matrices including breath [129], saliva [130], heart tissue, and urine [131], plasma, tissue, and cell culture lysates [26].

Chromatographic methods used in H_2S analysis include:

- i) GC coupled to different detectors as electrochemical [132], electron capture [133], flame photometry [134], mass spectrometry [135,136], ion mobility spectrometry [137].
- ii) LC coupled to different detectors as spectrophotometry [138], spectrofluorimetry [139], atomic fluorescence spectrometry [140], mass spectrometry [141], and electrochemical [142].

These chromatographic coupled techniques represent the most used chromatographic methods for H_2S analysis. However, these coupled techniques were used for different applications i.e., ion chromatography coupled to electrochemical detector was used for sulfide determination in water [143], in rat and human brain tissue [144], in rat brain different regions (brainstem, cerebellum hippocampus, striatum, and cortex) [145], in its liberation by the dithiothreitol treatment of brain tissue [146], in organic-rich, anaerobic waters from peat bogs [147], and in gastrointestinal contents and whole blood [142].

Generally, pre-column derivatization, (i.e., with methylene blue, pentafluorobenzyl bromide, etc) is required for H_2S detection. Therefore, during the derivatization step, the biomolecule-bound sulfur pool presents significant interferences during the analysis of biological samples alongside rigorous analytical precautions to be followed [22,148]

H_2S exists either in a gaseous state (unionized form) or liquid phase (unionized and two ionized forms). Unionized H_2S could be directly trapped (gaseous state) or liberated from its liquid phase in the headspace above the sample and was then directly analyzed by GC coupled to different detectors, as flame photometry and sulfur chemiluminescence detection. While H_2S in the liquid phase generally needs precolumn derivatization followed by GC or LC analysis [149]. Table 3 summarizes the analysis of sulfide using different chromatographic methods. Gas chromatographic analysis of sulfides was initially carried out via its pentafluorobenzyl derivative detection using mass spectrometry [150]. This technique was applied to post mortem analysis in forensic studies for

Table 3
Representative examples of certain chromatographic methods for H₂S analysis.

Chromatographic method	Properties and applications	Ref.
1 Ion-interaction RP-HPLC / spectrophotometry	Adv.: relatively simple protocol (methylene blue formation) Disadv.: need pre-column derivatization of sulfide, affect acid-labile sulfides Application: brain tissue and rumen fluid of cattle	[138]
2 Micro distillation/ ion chromatography / fluorescence detection	Adv.: acceptable recoveries (94–101%) Disadv.: low sensitivity (2.5 μM), non-selective for free sulfides (bound form/acid-labile), long preparation time (3 hrs/50°C) Application: gut contents (0.2 to 2.8 μmol/g wet feces) and whole blood sulphide (10–100 μM).	[142]
3 RP-HPLC / fluorescence	Adv.: sensitive (0.02 pmol) Disadv.: need pre-column derivatization of sulfide with monobromobimane, long incubation time (30 min), long analysis time (~20 min) Application: plasma of mice	[26]
4 RP-HPLC/mass spectrometry (ESI)	Adv.: good linear range 1–1000 nM, uses a novel stable isotope-coded (2-iodoacetanilide) Disadv.: used precolumn derivatizing agent (2-iodoacetanilide) Application: HepG2 (750 μM) cells <i>in vitro</i>	[141]
5 Gas dialysis/Ion chromatography/ electrochemical detection	Adv.: 95–99% Recovery Disadv.: need gas dialysis pretreatment, post-mortem analysis & couldn't be applied for real-time monitoring Application: rat and human brain	[144]
6 HS-GC-MS (EI)	Adv.: generation of H ₂ S in hermetically closed GC headspace vials, use a specific H ₂ S internal standard (N ₂ O), Disadv.: relative narrow linear range (12.5 – 62.5 μM), low sensitivity LOD (1 μM), at high concentration of CO ₂ , it coelutes with the internal standard (N ₂ O) & consequently affects H ₂ S quantification Application: quantify H ₂ S in H ₂ S fatal intoxication cases (post-mortem)	[178]
7 GC/MS (full scan)	Disadv.: requires a derivatization step and provide relatively not absolute amounts Application: blood (serum)	[136]
8 GC-MS (SIM mode)	Adv.: sensitive (96 ng/ml), linear range (10 – 100 μM) Disadv.: long incubation time (4 h) with a derivatizing agent (pentafluorobenzyl bromide), the possibility of interference of GSH & sulfur-containing amino acids Application: whole blood, blood levels of sulphide of healthy controls (35–80 μM)	[93]
9 GC/sulfur chemiluminescence detection	Adv.: selective, sensitive (15 pg/injected sample), rapid analysis time (H ₂ S less than 2 min), linear range (0 – 14 ng/injected sample) Disadv.: time-consuming for sample preparation and GC run cycle. Application: artificially induced H ₂ S production in tissue homogenate	[179]

sulfide fatal toxicity [151] and to investigate blood sulfide as a marker of bowel fermentation processes [93]. Later on, sulfide analysis was achieved in the headspace for tissue homogenates [38] or post silylation in human sera [152]. GC-MS analysis of human breath revealed the contribution of H₂S in oral malodor and halitosis [129]. Moreover, GC-MS analysis of human serum revealed elevation of H₂S level in a certain serious type of heart attack (ST-elevation myocardial infarction) [152].

A coupling electrochemical detector (ECD) with ion chromatography (IC) was applied for the determination of the sulfide in brain tissue. However, the main limitation resides in the liberation of the acid-labile sulfur during the high acidic extraction protocol [22]. Another example of IC coupled to ECD was investigating the protein-rich diet effect on sulfide level in the gut contents and whole blood [142]. Monobromobimane was the derivatizing agent for H₂S in alkaline medium (pH 9.5) and analyzed by HPLC coupled with fluorescence detection which offers good sensitivity compared to that obtained with the methylene blue method [26], whereas *via* coupling with a mass spectrometer, (ESI-MS), it surpasses other methods concerning sensitivity and specificity [141].

A validated liquid chromatography-mass spectrometry (LC-MS/MS) method for the determination of H₂S in various biological matrices by determination of a derivative of hydrogen sulfide and monobromobimane named sulfide dibimane (SDB) was used to measure its levels in a broad range of biological matrices, such as blood, plasma, tissues, cells, and enzymes, across different species [153]. The later technique revealed diurnal H₂S fluctuations in mice plasma [154].

Our aim in this review is not though to provide an inclusive overview of all chromatographic methods used in the assessment of biological H₂S, but rather to highlight certain examples of chromatographic techniques available as tools for its determination.

Electrochemical determination of H₂S

Electrochemical methods offer an improved expedited route for real-time detection of H₂S in biological samples due to their low detection limit, high sensitivity and selectivity, miniaturization capabilities, fast response time, and absence of chemical reagents [21]. Among different types of electrochemical sensors, potentiometric ion-selective electrodes and polarographic sensors have been employed extensively for H₂S determination in biological samples.

Ag/Ag₂S ion-selective electrode (ISE) is one of the most commonly used potentiometric methods for measuring sulfide ion in biological systems. This method was first reported fifty years ago by Mason et al. for measuring sulfide concentration in plasma with limited details of the methodology [155]. A full detailed procedure for plasma sulfide concentrations measurement using this electrode was later reported by Khan et al. [156]. Orion Research used this method to develop a commercial sulfide sensitive electrode (Model 9616, Orion Research, Beverly, MA) that has been widely used in serum H₂S measurement [157]. Interestingly, Lazar Research Laboratories (Los Angeles, CA) has developed another small commercial Ag/Ag₂S ISE known as ArrowH₂S™ that measures H₂S in volumes down to 10 μl directly in its micro containers with 100 nM detection limit, thus preventing H₂S loss from the sample and increasing the accuracy of its measurement [7]. However, Ag/Ag₂S electrodes exhibit some disadvantages such as the requirement for rendering the medium alkaline via adding “antioxidant buffer” to shift the H₂S equilibrium into the S²⁻ ions which are the only form of H₂S that the electrode can measure [158,159]. Besides, the electrode must be reconditioned (typically for 1 h in 5 mM Na₂S) to ensure that no silver is exposed to the surface otherwise, selectivity is lost [160]. Other potentiometric sulfide sensors based on the reversible electrochemical reaction of a redox mediator *viz.*, ferricyanide and conductive polymer as sensing film

have been also reported [161,162]. These methods exhibit high reproducibility and sensitivity.

Polarography is another reliable electrochemical technique that has been applied for the determination of H₂S in whole blood and tissues [21]. It has the advantage of real-time monitoring even for free H₂S gas without altering the sample. The first polarographic sensor used for H₂S determination in biological samples is based on a Clark-type oxygen electrode [163]. Platinum wires were used as the anode and cathode altogether with an alkaline K₃[Fe(CN)₆] as an internal electrolyte solution held in the sensor tip reservoir using H₂S-permeable membrane and a sensor housing of polyether ether ketone. During H₂S measurement, [Fe(CN)₆]³⁻ is reduced to [Fe(CN)₆]⁴⁻ while H₂S gas is oxidized to HS⁻ then S⁰ upon its permeation through the membrane layers. A current proportional to H₂S concentration is produced upon electrochemical oxidation of [Fe(CN)₆]⁴⁻ back into [Fe(CN)₆]³⁻ on the surface of the platinum electrode. Following this sensor, another miniature polarographic H₂S sensor was developed having several advantages including sensitive detection limit (10 nM) and low response time (20–30 s) posing it as an ideal sensor for kinetic studies of H₂S metabolism in broken cell systems, intact tissues, and whole organisms [164]. Moreover, the sensor could be combined with other real-time polarographic sensors such as polarographic oxygen sensor and polarographic nitric oxide sensor owing to its higher selectivity to determine the correlation of these species with H₂S in biological systems. Additionally, an ultra-micro polarographic H₂S sensor having a diameter of only 100 μm has been developed offering several advantages, including durability for long-term use, rapid response time, and absence of sleeves and filling solutions [21]. Despite the numerous advantages for H₂S polarographic sensors as one of the widely used techniques for real-time H₂S measurement, their main disadvantage lies in the necessity of liquid electrolytes in their design which are prone to dryness and leakage in addition to the possible large residual current associated with impurities in the samples.

Conclusion

Owing to the major clinical importance of H₂S as the third gasotransmitter, a wide variety of quantification methods have been developed for its measurement in biological systems. In contrast to colorimetric, ion-selective electrodes, and chromatographic methods, fluorescence offers an attractive non-invasive and promising approach accounting for the substantial increase in the number of newly developed fluorescent probes in the past few years. Although a lot of effort has been made towards fluorescence imaging, it faces challenges such as the low levels of endogenous H₂S and the presence of many interfering biomolecules. Besides, tissue penetration, fluorophore stability at high excitation wavelengths have also largely limited their application for *in vivo* H₂S quantification. Although fluorescence sensors offer good selectivity they cannot be considered as H₂S-specific probes, as biothiols may interact, even at a lesser extent, with these sensors. Consequently, significant work has to be done towards developing highly sensitive and selective fluorescent probes for such purpose. Promising fluorescent probes, for monitoring the endogenous short-lived H₂S, are expected to meet certain requirements, such as a photostability, NIR optical window, enhanced fluorescence, fast and sensitive response, specificity or high selectivity, water solubility and low cytotoxicity. On the other hand, colorimetric assays are among the earliest and most common methods used for *in vitro* H₂S detection, however, their employment *in vivo* H₂S measurement has not yet been possible even after the introduction of plasmonic metal nanoparticles that have provided an expedited route for rapid and accurate detec-

tion of H₂S in plasma. Separation techniques as gas or liquid chromatography offer higher selectivity compared to direct spectrophotometric or fluorescence H₂S measurements, albeit they also could not be applied for H₂S real-time monitoring. These methods are suitable for endpoint measurements i.e. plasma or tissue samples. Despite a myriad of developed analytical procedures used for H₂S determination, the need for highly selective, highly sensitive, biocompatible, reproducible, and accurate H₂S measurement methods seems imperative to untangle the non-resolved pitfalls of the current methods.

Compliance with ethics requirements

This article does not contain any studies with human or animal subjects

Declaration of Competing Interest

The authors have declared no conflict of interest.

Acknowledgment

Dr. Farag thanks Jesour grant number 30, Academy of Scientific Research and Technology, ASRT, Egypt for funding.

References

- [1] Zheng Y, Yu B, De La Cruz LK, Roy Choudhury M, Anifowose A, Wang B. Toward Hydrogen Sulfide Based Therapeutics: Critical Drug Delivery and Developability Issues. *Med Res Rev* 2018;38(1):57–100.
- [2] Li L, Moore P. Putative biological roles of hydrogen sulfide in health and disease: a breath of not so fresh air?. *Trends Pharmacol Sci* 2008;29(2):84–90.
- [3] Kimura H. Hydrogen sulfide as a neuromodulator. *Mol Neurobiol* 2002;26(1):13–9.
- [4] Cunha TM, Dal-Secco D, Verri WA, Guerrero AT, Souza GR, Vieira SM, et al. Dual role of hydrogen sulfide in mechanical inflammatory hypernociception. *Eur J Pharmacol* 2008;590(1):127–35.
- [5] Elrod JW, Calvert JW, Morrison J, Doeller JE, Kraus DW, Tao L, et al. Hydrogen sulfide attenuates myocardial ischemia-reperfusion injury by preservation of mitochondrial function. *Proc Natl Acad Sci* 2007;104(39):15560–5.
- [6] Yang G, Wu L, Jiang B, Yang W, Qi J, Cao K, et al. H₂S as a physiologic vasorelaxant: hypertension in mice with deletion of cystathionine gamma-lyase. *Science* (New York, NY) 2008;322(5901):587–90.
- [7] Yang G, Wu L, Jiang B, Yang W, Qi J, Cao K, et al. H₂S as a Physiologic Vasorelaxant: Hypertension in Mice with Deletion of Cystathionine γ-Lyase. *Science* 2008;322(5901):587–90.
- [8] Kimura H. Hydrogen Sulfide: From Brain to Gut. *Antioxid Redox Signal* 2009;12(9):1111–23.
- [9] Hu L-F, Lu M, Tiong CX, Dawe GS, Hu G, Bian J-S. Neuroprotective effects of hydrogen sulfide on Parkinson's disease rat models. *Aging Cell* 2010;9(2):135–46.
- [10] Eto K, Asada T, Arima K, Makifuchi T, Kimura H. Brain hydrogen sulfide is severely decreased in Alzheimer's disease. *Biochem Biophys Res Commun* 2002;293(5):1485–8.
- [11] Kamoun P, Belardinelli M-C, Chabli A, Lallouchi K, Chadefaux-Vekemans B. Endogenous hydrogen sulfide overproduction in Down syndrome. *American Journal of Medical Genetics Part A* 2003;116A(3):310–1.
- [12] Jain SK, Bull R, Rains JL, Bass PF, Levine SN, Reddy S, et al. Low levels of hydrogen sulfide in the blood of diabetes patients and streptozotocin-treated rats causes vascular inflammation?. *Antioxid Redox Signal* 2010;12(11):1333–7.
- [13] Hughes MN, Centelles MN, Moore KP. Making and working with hydrogen sulfide: The chemistry and generation of hydrogen sulfide *in vitro* and its measurement *in vivo*: A review. *Free Radical Biol Med* 2009;47(10):1346–53.
- [14] Nagy P, Pálinskás Z, Nagy A, Budai B, Tóth I, Vasas A: Chemical aspects of hydrogen sulfide measurements in physiological samples. *Biochimica et Biophysica Acta (BBA)-General Subjects* 2014;1840(2):876–91.
- [15] Alyan AK, Hanafi RS, Gad MZ. Point-of-care testing and optimization of sample treatment for fluorometric determination of hydrogen sulphide in plasma of cardiovascular patients. *J Adv Res* 2021;27:1–10.
- [16] Shen X, Peter EA, Bir S, Wang R, Kevill CG. Analytical measurement of discrete hydrogen sulfide pools in biological specimens. *Free Radical Biol Med* 2012;52(11–12):2276–83.
- [17] Cao X, Ding L, Xie Z-z, Yang Y, Whiteman M, Moore PK, Bian J-S: A review of hydrogen sulfide synthesis, metabolism, and measurement: is modulation of hydrogen sulfide a novel therapeutic for cancer?. *Antioxid Redox Signal* 2019;31(1):1–38.

- [18] Amilan Jose D, Sharma N, Sakla R, Kaushik R, Gadiyaram S. Fluorescent nanoprobe for the sensing of gasotransmitters hydrogen sulfide (H₂S), nitric oxide (NO) and carbon monoxide (CO). *Methods* 2019;168:62–75.
- [19] Luo Y, Zhu C, Du D, Lin Y. A review of optical probes based on nanomaterials for the detection of hydrogen sulfide in biosystems. *Anal Chim Acta* 2019;1061:1–12.
- [20] Vitvitsky V, Banerjee R: Chapter Seven - H₂S Analysis in Biological Samples Using Gas Chromatography with Sulfur Chemiluminescence Detection. In: *Methods in Enzymology*. Edited by Cadenas E, Packer L, vol. 554: Academic Press; 2015: 111-123.
- [21] Xu T, Scafa N, Xu L-P, Zhou S, Abdullah Al-Ghanem K, Mahboob S, et al. Electrochemical hydrogen sulfide biosensors. *Analyst* 2016;141(4):1185–95.
- [22] Ubuka T. Assay methods and biological roles of labile sulfur in animal tissues. *J Chromatogr B* 2002;781(1):227–49.
- [23] Kumar N, Bhalla V, Kumar M. Recent developments of fluorescent probes for the detection of gasotransmitters (NO, CO and H₂S). *Coord Chem Rev* 2013;257(15):2335–47.
- [24] Xiong B, Peng L, Cao X, He Y, Yeung ES. Optical analysis of biological hydrogen sulphide: an overview of recent advancements. *Analyst* 2015;140(6):1763–71.
- [25] Pandey SK, Kim K-H, Tang K-T. A review of sensor-based methods for monitoring hydrogen sulfide. *TrAC, Trends Anal Chem* 2012;32:87–99.
- [26] Shen X, Pattillo CB, Pardue S, Bir SC, Wang R, Kevill CG. Measurement of plasma hydrogen sulfide in vivo and in vitro. *Free Radical Biol Med* 2011;50(9):1021–31.
- [27] Yi L, Xi Z. Thiolytic of NBD-based dyes for colorimetric and fluorescence detection of H₂S and biothiols: design and biological applications. *Org Biomol Chem* 2017;15(18):3828–39.
- [28] Li J, Yin C, Huo F. Chromogenic and fluorogenic chemosensors for hydrogen sulfide: review of detection mechanisms since the year 2009. *RSC Adv* 2015;5(3):2191–206.
- [29] Vikrant K, Kumar V, Ok YS, Kim K-H, Deep A. Metal-organic framework (MOF)-based advanced sensing platforms for the detection of hydrogen sulfide. *TrAC, Trends Anal Chem* 2018;105:263–81.
- [30] Yu F, Han X, Chen L. Fluorescent probes for hydrogen sulfide detection and bioimaging. *Chem Commun* 2014;50(82):12234–49.
- [31] Kaushik R, Ghosh A, Amilan Jose D. Recent progress in hydrogen sulphide (H₂S) sensors by metal displacement approach. *Coord Chem Rev* 2017;347:141–57.
- [32] Tangerman A. Measurement and biological significance of the volatile sulfur compounds hydrogen sulfide, methanethiol and dimethyl sulfide in various biological matrices. *J Chromatogr B* 2009;877(28):3366–77.
- [33] Luo Y, Zhu C, Du D, Lin Y. A review of optical probes based on nanomaterials for the detection of hydrogen sulfide in biosystems. *Anal Chim Acta* 2019.
- [34] Ma Y, Wang H, Su S, Chen Y, Li Y, Wang X, et al. A red mitochondria-targeted AlEgen for visualizing H₂S in living cells and tumours. *Analyst* 2019;144(10):3381–8.
- [35] Montoya LA, Pluth MD. Organelle-targeted H₂S probes enable visualization of the subcellular distribution of H₂S donors. *Anal Chem* 2016;88(11):5769–74.
- [36] Gao P, Pan W, Li N, Tang B. Fluorescent probes for organelle-targeted bioactive species imaging. *Chem Sci* 2019;10(24):6035–71.
- [37] Sunzini F, De Stefano S, Chimenti MS, Melino S. Hydrogen sulfide as potential regulatory gasotransmitter in arthritic diseases. *Int J Mol Sci* 2020;21(4):1180.
- [38] Furne J, Saeed A, Levitt MD. Whole tissue hydrogen sulfide concentrations are orders of magnitude lower than presently accepted values. *American Journal of Physiology-Regulatory, Integrative and Comparative Physiology* 2008;295(5):R1479–85.
- [39] Peng X, Song F, Lu E, Wang Y, Zhou W, Fan J, et al. Heptamethine cyanine dyes with a large Stokes shift and strong fluorescence: a paradigm for excited-state intramolecular charge transfer. *J Am Chem Soc* 2005;127(12):4170–1.
- [40] Lippert AR, New EJ, Chang CJ. Reaction-based fluorescent probes for selective imaging of hydrogen sulfide in living cells. *J Am Chem Soc* 2011;133(26):10078–80.
- [41] Wang R, Yu F, Chen L, Chen H, Wang L, Zhang W. A highly selective turn-on near-infrared fluorescent probe for hydrogen sulfide detection and imaging in living cells. *Chem Commun* 2012;48(96):11757–9.
- [42] Xuan W, Pan R, Cao Y, Liu K, Wang W. A fluorescent probe capable of detecting H₂S at submicromolar concentrations in cells. *Chem Commun* 2012;48(86):10669–71.
- [43] Chen J, Zhao M, Jiang X, Sizovs A, Wang MC, Provost CR, et al. Genetically anchored fluorescent probes for subcellular specific imaging of hydrogen sulfide. *Analyst* 2016;141(4):1209–13.
- [44] Yang S, Qi Y, Liu C, Wang Y, Zhao Y, Wang L, et al. Design of a simultaneous target and location-activatable fluorescent probe for visualizing hydrogen sulfide in lysosomes. *Anal Chem* 2014;86(15):7508–15.
- [45] Qiao Z, Zhang H, Wang K, Zhang Y. A highly sensitive and responsive fluorescent probe based on 6-azide-chroman dye for detection and imaging of hydrogen sulfide in cells. *Talanta* 2019;195:850–6.
- [46] Kang N, Pei S, Zhang C, Zhang G, Zhou Y, Shi L, et al. A turn-on fluorescence probe for hydrogen sulfide in absolute aqueous solution. *Spectrochimica Acta Part A: Molecular and Biomolecular Spectroscopy*; 2020. p. 118156.
- [47] Peng H, Cheng Y, Dai C, King AL, Predmore BL, Lefer DJ, et al. A fluorescent probe for fast and quantitative detection of hydrogen sulfide in blood. *Angew Chem Int Ed* 2011;50(41):9672–5.
- [48] Zhang Y, Zhang L. A novel "turn-on" fluorescent probe based on hydroxy functionalized naphthalimide as a logic platform for visual recognition of H₂S in environment and living cells. *Spectrochimica Acta Part A: Molecular and Biomolecular Spectroscopy*; 2020. p. 118331.
- [49] Yu C, Li X, Zeng F, Zheng F, Wu S. Carbon-dot-based ratiometric fluorescent sensor for detecting hydrogen sulfide in aqueous media and inside live cells. *Chem Commun* 2013;49(4):403–5.
- [50] Kim M, Seo YH, Kim Y, Heo J, Jang W-D, Sim SJ, et al. A fluorogenic molecular nanoprobe with an engineered internal environment for sensitive and selective detection of biological hydrogen sulfide. *Chem Commun* 2017;53(14):2275–8.
- [51] Shen D, Liu J, Sheng L, Lv Y, Wu G, Wang P, et al. Design, synthesis and evaluation of a novel fluorescent probe to accurately detect H₂S in hepatocytes and natural waters. *Spectrochimica Acta Part A: Molecular and Biomolecular Spectroscopy*; 2019. p. 117690.
- [52] Ji A, Fan Y, Ren W, Zhang S, Ai H-w. A sensitive near-infrared fluorescent sensor for mitochondrial hydrogen sulfide. *ACS Sensors* 2018;3(5):992–7.
- [53] Paul N, Sarkar R, Sarkar R, Barui A, Sarkar S. Detection of hydrogen sulfide using BODIPY based colorimetric and fluorescent on-off chemosensor. *J Chem Sci* 2020;132(1):21.
- [54] Yi X, Liu M, Luo Q, Zhuo H, Cao H, Wang J, et al. Toxic effects of dimethyl sulfoxide on red blood cells, platelets, and vascular endothelial cells in vitro. *FEBS Open Bio* 2017;7(4):485–94.
- [55] Chi L-M, Wu W-g. Mechanism of hemolysis of red blood cell mediated by ethanol. *Biochimica et Biophysica. Acta (BBA)-Biomembranes* 1991;1062(1):46–50.
- [56] Yu F, Li P, Song P, Wang B, Zhao J, Han K. An ICT-based strategy to a colorimetric and ratiometric fluorescence probe for hydrogen sulfide in living cells. *Chem Commun* 2012;48(23):2852–4.
- [57] Noudeh GD, Khazaeli P, Rahmani P. Study of the effects of polyethylene glycol sorbitan esters surfactants group on biological membranes. *Int J Pharmacol* 2008;4(1):27–33.
- [58] Karunya R, Jayaprakash K, Gaikwad R, Sajeesh P, Ramshad K, Muraleedharan K, et al. Rapid measurement of hydrogen sulphide in human blood plasma using a microfluidic method. *Sci Rep* 2019;9(1):1–11.
- [59] Lin X, Lu X, Zhou J, Ren H, Dong X, Zhao W, et al. Instantaneous fluorescent probe for the specific detection of H₂S. *Spectrochim Acta Part A Mol Biomol Spectrosc* 2019;213:416–22.
- [60] Liu J, Chen X, Zhang Y, Gao G, Zhang X, Hou S. A novel xanthene-based colorimetric and fluorescence probe for detection of H₂S in living cells. *J Lumin* 2018;204:480–4.
- [61] Wang H, Hu L, Xu B, Chen H, Cai F, Yang N, et al. Endoplasmic reticulum-targeted fluorogenic probe based on pyrimidine derivative for visualizing exogenous/endogenous H₂S in living cells. *Dyes Pigm* 2020;108390.
- [62] Li N, Than A, Chen J, Xi F, Liu J, Chen P. Graphene quantum dots based fluorescence turn-on nanoprobe for highly sensitive and selective imaging of hydrogen sulfide in living cells. *Biomater Sci* 2018;6(4):779–84.
- [63] Hong J, Feng W, Feng G. Highly selective near-infrared fluorescent probe with rapid response, remarkable large Stokes shift and bright fluorescence for H₂S detection in living cells and animals. *Sens Actuators, B* 2018;262:837–44.
- [64] Yang B, Su M-M, Xue Y-S, He Z-X, Xu C, Zhu H-L. A selective fluorescence probe for H₂S from biothiols with a significant regioselective turn-on response and its application for H₂S detection in living cells and in living *Caenorhabditis elegans*. *Sens Actuators, B* 2018;276:456–65.
- [65] Feng S, Xia Q, Feng G. Iminocoumarin-based red to near-infrared fluorescent turn-on probe with a large Stokes shift for imaging H₂S in living cells and animals. *Dyes Pigm* 2019;163:447–53.
- [66] Huang Y, Zhang C, Xi Z, Yi L. Synthesis and characterizations of a highly sensitive and selective fluorescent probe for hydrogen sulfide. *Tetrahedron Lett* 2016;57(10):1187–91.
- [67] Wu M-X, Sha X-L, Wei X-R, Sun R, Chen Y, Gao J, et al. Fluorescent hydrogen sulfide probes based on azonia-cyanine dyes and their imaging applications in organelles. *Anal Chim Acta* 2019;1068:60–9.
- [68] Wang R, Li Z, Zhang C, Li Y, Xu G, Zhang QZ, et al. Fast-Response Turn-on Fluorescent Probes Based on Thiolytic of NBD Amine for H₂S Bioimaging. *ChemBioChem* 2016;17(10):962–8.
- [69] Wang Y, Lv X, Guo W. A reaction-based and highly selective fluorescent probe for hydrogen sulfide. *Dyes Pigm* 2017;139:482–6.
- [70] Gu X-H, Lei Y, Wang S, Cao F, Zhang Q, Chen S, et al. Tetrahydro [5] helicene fused nitrobenzoxadiazole as a fluorescence probe for hydrogen sulfide, cysteine/homocysteine and glutathione. *Spectrochim Acta Part A Mol Biomol Spectrosc* 2020;229:118003.
- [71] Pak YL, Li J, Ko KC, Kim G, Lee JY, Yoon J. Mitochondria-targeted reaction-based fluorescent probe for hydrogen sulfide. *Anal Chem* 2016;88(10):5476–81.
- [72] Wei C, Wei L, Xi Z, Yi L. A FRET-based fluorescent probe for imaging H₂S in living cells. *Tetrahedron Lett* 2013;54(50):6937–9.
- [73] Qian Y, Karpus J, Kabil O, Zhang S-Y, Zhu H-L, Banerjee R, et al. Selective fluorescent probes for live-cell monitoring of sulphide. *Nat Commun* 2011;2:495.
- [74] Samanta SK, Ali SS, Gangopadhyay A, Maiti K, Pramanik AK, Guria UN, et al. A highly selective ratiometric fluorescent probe for H₂S based on new heterocyclic ring formation and detection in live cells. *Supramol Chem* 2019;31(5):349–60.

- [75] Chao J, Xu M, Zhang Y, Huo F, Liu Y, Wang X, et al. HS– facilitated sulfur pyran realizing hydrogen sulfide detection and imaging in HepG2 cells and chlorella. *Spectrochim Acta Part A Mol Biomol Spectrosc* 2019;214:227–32.
- [76] Men J, Yang X, Zhang H, Zhou J. A near-infrared fluorescent probe based on nucleophilic substitution–cyclization for selective detection of hydrogen sulfide and bioimaging. *Dyes Pigm* 2018;153:206–12.
- [77] Zhang X, Qu W, Liu H, Ma Y, Wang L, Sun Q, et al. Visualizing hydrogen sulfide in living cells and zebrafish using a red-emitting fluorescent probe via selenium–sulfur exchange reaction. *Anal Chim Acta* 2020.
- [78] Liu C, Pan J, Li S, Zhao Y, Wu LY, Berkman CE, et al. Capture and visualization of hydrogen sulfide by a fluorescent probe. *Angew Chem Int Ed* 2011;50(44):10327–9.
- [79] Forman HJ, Zhang H, Rinna A. Glutathione: overview of its protective roles, measurement, and biosynthesis. *Mol Aspects Med* 2009;30(1–2):1–12.
- [80] Wang J, Wen Y, Huo F, Yin C. Based 'successive' nucleophilic substitution mitochondrial-targeted H2S red light emissive fluorescent probe and its imaging in mice. *Sens Actuators, B* 2019;297:126773.
- [81] Liu Z, Liu L, Li J, Qin Y, Zhao C, Mi Y, et al. A new coumarin-based fluorescent probe for selective recognition of Cu²⁺ and S²⁻ in aqueous solution and living cells. *Tetrahedron* 2019.
- [82] Kaushik R, Kumar P, Ghosh A, Gupta N, Kaur D, Arora S, et al. Alizarin red S–zinc (ii) fluorescent ensemble for selective detection of hydrogen sulphide and assay with an H₂S donor. *RSC Adv* 2015;5(97):79309–16.
- [83] Santos-Figueroa LE, de la Torre C, El Sayed S, Sancenón F, Martínez-Mañez R, Costero AM, et al. Highly Selective Fluorescence Detection of Hydrogen Sulfide by Using an Anthracene-Functionalized Cyclam–Cull Complex. *Eur J Inorg Chem* 2014;2014(1):41–5.
- [84] Luo Y, Song Y, Zhu C, Li S, Xian M, Wai CM, et al. Visualization of endogenous hydrogen sulfide in living cells based on Au nanorods@ silica enhanced fluorescence. *Anal Chim Acta* 2019;1053:81–8.
- [85] Wang C, Ding Y, Bi X, Luo J, Wang G, Lin Y. Carbon quantum dots–Ag nanoparticle complex as a highly sensitive “turn-on” fluorescent probe for hydrogen sulfide: a DFT/TD-DFT study of electronic transitions and mechanism of sensing. *Sens Actuators, B* 2018;264:404–9.
- [86] Gao P, Li M, Zhang Y, Dong C, Zhang G, Shi L, et al. Facile, rapid one-pot synthesis of multifunctional gold nanoclusters for cell imaging, hydrogen sulfide detection and pH sensing. *Talanta* 2019;197:1–11.
- [87] Au-Yeung HY, Chan CY, Tong KY, Yu ZH. Copper-based reactions in analyte-responsive fluorescent probes for biological applications. *J Inorg Biochem* 2017;177:300–12.
- [88] DeLeon ER, Stoy GF, Olson KR. Passive loss of hydrogen sulfide in biological experiments. *Anal Biochem* 2012;421(1):203–7.
- [89] Zaorska E, Tomasova L, Koszelewski D, Ostaszewski R, Ufnal M. Hydrogen Sulfide in Pharmacotherapy, Beyond the Hydrogen Sulfide-Donors. *Biomolecules* 2020;10(2):323.
- [90] Li Q, Lancaster Jr JR. Chemical foundations of hydrogen sulfide biology. *Nitric Oxide* 2013;35:21–34.
- [91] Kaushik R, Ghosh A, Jose DA. Recent progress in hydrogen sulphide (H₂S) sensors by metal displacement approach. *Coord Chem Rev* 2017;347:141–57.
- [92] Gu X, Liu C, Zhu Y-C, Zhu Y-Z. Development of a boron–dipyromethene–Cu²⁺ ensemble based colorimetric probe toward hydrogen sulfide in aqueous media. *Tetrahedron Lett* 2011;52(39):5000–3.
- [93] Rr Hyšpler, Tichá A, Indrová M, Zadák Z, Hyšplerová L, Gasparič J, Churáček J: A simple, optimized method for the determination of sulphide in whole blood by GC–MS as a marker of bowel fermentation processes. *J Chromatogr B* 2002;770(1–2):255–9.
- [94] Zhong K, Chen L, Pan Y, Yan X, Hou S, Tang Y, et al. A colorimetric and near-infrared fluorescent probe for detection of hydrogen sulfide and its real multiple applications. *Spectrochim Acta Part A Mol Biomol Spectrosc* 2019;221:117135.
- [95] Kaushik R, Ghosh A, Singh A, Jose DA. Colorimetric sensor for the detection of H₂S and its application in molecular half-subtractor. *Anal Chim Acta* 2018;1040:177–86.
- [96] Fischer E. Bildung von Methylenblau als Reaktion auf Schwefelwasserstoff. *Ber Dtsch Chem Ges* 1883;16(2):2234–6.
- [97] Fogo JK, Popowsky M. Spectrophotometric Determination of Hydrogen Sulfide. *Anal Chem* 1949;21(6):732–4.
- [98] Montoya LA, Pearce TF, Hansen RJ, Zakharov LN, Pluth MD. Development of Selective Colorimetric Probes for Hydrogen Sulfide Based on Nucleophilic Aromatic Substitution. *The Journal of Organic Chemistry* 2013;78(13):6550–7.
- [99] Zhang D, Jin W. Highly selective and sensitive colorimetric probe for hydrogen sulfide by a copper (II) complex of azo-dye based on chemosensing ensemble approach. *Spectrochim Acta Part A Mol Biomol Spectrosc* 2012;90:35–9.
- [100] Carpenter TS, Rosolina SM, Xue Z-L. Quantitative, colorimetric paper probe for hydrogen sulfide gas. *Sens Actuators, B* 2017;253:846–51.
- [101] Jarosz AP, Yep T, Mutus B. Microplate-Based Colorimetric Detection of Free Hydrogen Sulfide. *Anal Chem* 2013;85(7):3638–43.
- [102] Ahn YJ, Lee YJ, Lee J, Lee D, Park H-K, Lee G-J. Colorimetric detection of endogenous hydrogen sulfide production in living cells. *Spectrochim Acta Part A Mol Biomol Spectrosc* 2017;177:118–24.
- [103] Zhang Y, Shen H-Y, Hai X, Chen X-W, Wang J-H. Polyhedral Oligomeric Silesquioxane Polymer-Caged Silver Nanoparticle as a Smart Colorimetric Probe for the Detection of Hydrogen Sulfide. *Anal Chem* 2017;89(2):1346–52.
- [104] Yang X, Ren Y, Gao Z. Silver/Gold Core-Shell Nanoprism-Based Plasmonic Nanoprobes for Highly Sensitive and Selective Detection of Hydrogen Sulfide. *Chemistry – A European Journal* 2015;21(3):988–92.
- [105] Zeng J, Li M, Liu A, Feng F, Zeng T, Duan W, et al. Au/Ag₂ Dimeric Nanoparticles for Highly Selective and Sensitive Colorimetric Detection of Hydrogen Sulfide. *Adv Funct Mater* 2018;28(26):1800515.
- [106] Zhang J, Xu X, Yang X. Highly specific colorimetric recognition and sensing of sulfide with glutathione-modified gold nanoparticle probe based on an anion-for-molecule ligand exchange reaction. *Analyst* 2012;137(7):1556–8.
- [107] Zhang X, Zhou W, Yuan Z, Lu C. Colorimetric detection of biological hydrogen sulfide using fluorosurfactant functionalized gold nanorods. *Analyst* 2015;140(21):7443–50.
- [108] Gao Z, Tang D, Tang D, Niessner R, Knopp D. Target-Induced Nanocatalyst Deactivation Facilitated by Core@Shell Nanostructures for Signal-Amplified Headspace-Colorimetric Assay of Dissolved Hydrogen Sulfide. *Anal Chem* 2015;87(19):10153–60.
- [109] Yang Y, Zhao Q, Feng W, Li F. Luminescent Chemodosimeters for Bioimaging. *Chem Rev* 2013;113(1):192–270.
- [110] You Y. Phosphorescence bioimaging using cyclometalated Ir(III) complexes. *Curr Opin Chem Biol* 2013;17(4):699–707.
- [111] Yu Q, Zhang KY, Liang H, Zhao Q, Yang T, Liu S, et al. Dual-Emissive Nanohybrid for Ratiometric Luminescence and Lifetime Imaging of Intracellular Hydrogen Sulfide. *ACS Appl Mater Interfaces* 2015;7(9):5462–70.
- [112] Wu P, Zhang J, Wang S, Zhu A, Hou X. Sensing during In Situ Growth of Mn-Doped ZnS QDs: A Phosphorescent Sensor for Detection of H₂S in Biological Samples. *Chemistry – A European Journal* 2014;20(4):952–6.
- [113] Lee JS, Joung H-A, Kim M-G, Park CB. Graphene-Based Chemiluminescence Resonance Energy Transfer for Homogeneous Immunoassay. *ACS Nano* 2012;6(4):2978–83.
- [114] Zhang L, Rong W, Lu C, Zhao L. Organo-modified layered double hydroxide-catalyzed Fenton-like ultra-weak chemiluminescence for specific sensing of vitamin B12 in egg yolks. *Talanta* 2014;129:126–31.
- [115] Fang Z, Yue G, Wang J, Luo F, Guo L, Qiu B, et al. Chemiluminescent sensor for hydrogen sulfide in rat brain microdialysis based on target-induced horseradish peroxidase deactivation. *Anal Methods* 2019;11(24):3085–9.
- [116] Spencer Bailey T, Pluth MD: Chapter Five - Chemiluminescent Detection of Enzymatically Produced H₂S. In: *Methods in Enzymology*. Edited by Cadenas E, Packer L, vol. 554: Academic Press; 2015: 81–99.
- [117] Richter MM. Electrochemiluminescence (ECL). *Chem Rev* 2004;104(6):3003–36.
- [118] Park J, Kim T, Kim HJ, Hong J-I. Iridium(III) complex-based electrochemiluminescent probe for H₂S. *Dalton Trans* 2019;48(14):4565–73.
- [119] Zhang Y-Y, Zhou H, Wu P, Zhang H-R, Xu J-J, Chen H-Y. In Situ Activation of CdS Electrochemiluminescence Film and Its Application in H₂S Detection. *Anal Chem* 2014;86(17):8657–64.
- [120] Huang J, Qu W, Zhu J, Liu H, Wen W, Zhang X, et al. Electrochemiluminescent sensor based on Ru(bpy)₃²⁺-doped silica nanoprobe by incorporating a new co-reactant NBD-amine for selective detection of hydrogen sulfide. *Sens Actuators, B* 2019;284:451–5.
- [121] Zhang Z, Zhang S, Zhang X. Recent developments and applications of chemiluminescence sensors. *Anal Chim Acta* 2005;541(1):37–46.
- [122] Miao Z, Wu Y, Zhang X, Liu Z, Han B, Ding K, et al. Large-scale production of self-assembled SnO₂ nanospheres and their application in high-performance chemiluminescence sensors for hydrogen sulfide gas. *J Mater Chem* 2007;17(18):1791–6.
- [123] Zhang Z, Jiang H, Xing Z, Zhang X. A highly selective chemiluminescent H₂S sensor. *Sens Actuators, B* 2004;102(1):155–61.
- [124] Sun Z, Yuan H, Liu Z, Han B, Zhang X. A Highly Efficient Chemical Sensor Material for H₂S: α-Fe₂O₃ Nanotubes Fabricated Using Carbon Nanotube Templates. *Adv Mater* 2005;17(24):2993–7.
- [125] Jiang H, Hu J, Gu F, Shao W, Li C. Hydrothermal synthesis of novel In₂O₃ microspheres for gas sensors. *Chem Commun* 2009;24:3618–20.
- [126] Liu Y, Tang F, Kang CJ, Cao X. Detection of hydrogen sulphide using cataluminescence sensors based on alkaline-earth metal salts. *Luminescence* 2012;27(4):274–8.
- [127] Wan X, Wu L, Zhang L, Song H, Lv Y. Novel metal-organic frameworks-based hydrogen sulfide cataluminescence sensors. *Sens Actuators, B* 2015;220:614–21.
- [128] Wu L, Zhang L, Sun M, Liu R, Yu L, Lv Y. Metal-Free Cataluminescence Gas Sensor for Hydrogen Sulfide Based on Its Catalytic Oxidation on Silicon Carbide Nanocages. *Anal Chem* 2017;89(24):13666–72.
- [129] Van den Velde S, van Steenberghe D, Van Hee P, Quirynen M. Detection of odorless compounds in breath. *J Dent Res* 2009;88(3):285–9.
- [130] Solis MC, Volpe AR. Determination of Sulfur Volatiles in Putrefied Saliva by a Gas Chromatography–Microcoulometric Titrating System. *J Periodontol* 1973;44(12):775–8.
- [131] Jin S, Pu S-X, Hou C-L, Ma F-F, Li N, Li X-H, et al. Zhu Y-C: Cardiac H₂S generation is reduced in ageing diabetic mice. *Oxidative medicine and cellular longevity* 2015, 2015.
- [132] Kage S, Takekawa K, Kurosaki K, Imamura T, Kudo K. The usefulness of thiosulfate as an indicator of hydrogen sulfide poisoning: three cases. *Int J Legal Med* 1997;110(4):220–2.
- [133] Shigetoshi K, Nagata T, Kimura K, Kudo K. Extractive alkylation and gas chromatographic analysis of sulfide. *J Forensic Sci* 1988;33(1):217–22.

- [134] Radford-Knoery J, Cutter GA. Determination of carbonyl sulfide and hydrogen sulfide species in natural waters using specialized collection procedures and gas chromatography with flame photometric detection. *Anal Chem* 1993;65(8):976–82.
- [135] Suarez F, Furne J, Springfield J, Levitt MD. Morning breath odor: influence of treatments on sulfur gases. *J Dent Res* 2000;79(10):1773–7.
- [136] Ali SE, Farag MA, Holvoet P, Hanafi RS, Gad MZ. A comparative metabolomics approach reveals early biomarkers for metabolic response to acute myocardial infarction. *Sci Rep* 2016;6:36359.
- [137] Tiele A, Daly A, Hattersley J, Pinto A, Evans S, Ashmore C, et al. Investigation of paediatric PKU breath malodour, comparing glycomacropeptide with phenylalanine free L-amino acid supplements. *J Breath Res* 2019;14(1):016001.
- [138] Savage J, Gould D. Determination of sulfide in brain tissue and rumen fluid by ion-interaction reversed-phase high-performance liquid chromatography. *Journal of Chromatography, Biomedical Applications* 1990;526(2):540–5.
- [139] Wintner EA, Deckwerth TL, Langston W, Bengtsson A, Leviten D, Hill P, et al. A monobromobimane-based assay to measure the pharmacokinetic profile of reactive sulphide species in blood. *Br J Pharmacol* 2010;160(4):941–57.
- [140] Bramanti E, D'Ulivo L, Lomonte C, Onor M, Zamboni R, Raspi G, et al. Determination of hydrogen sulfide and volatile thiols in air samples by mercury probe derivatization coupled with liquid chromatography–atomic fluorescence spectrometry. *Anal Chim Acta* 2006;579(1):38–46.
- [141] Lee D-Y, Huang W-C, Gu T-J, Chang G-D. Quantitative and comparative liquid chromatography-electrospray ionization-mass spectrometry analyses of hydrogen sulfide and thiol metabolites derivatized with 2-iodoacetanilide isotopologues. *J Chromatogr A* 2018;1552:43–52.
- [142] Richardson CJ, Magee EA, Cummings JH. A new method for the determination of sulphide in gastrointestinal contents and whole blood by microdistillation and ion chromatography. *Clin Chim Acta* 2000;293(1–2):115–25.
- [143] Goodwin LR, Francom D, Urso A, Dieken FP. Determination of trace sulfides in turbid waters by gas dialysis/ion chromatography. *Anal Chem* 1988;60(3):216–9.
- [144] Goodwin LR, Francom D, Dieken FP, Taylor JD, Warenycia MW, Reiffenstein R, et al. Determination of sulfide in brain tissue by gas dialysis/ion chromatography: postmortem studies and two case reports. *J Anal Toxicol* 1989;13(2):105–9.
- [145] Warenycia MW, Goodwin LR, Benishin CG, Reiffenstein R, Francom DM, Taylor JD, et al. Acute hydrogen sulfide poisoning: demonstration of selective uptake of sulfide by the brainstem by measurement of brain sulfide levels. *Biochem Pharmacol* 1989;38(6):973–81.
- [146] Warenycia MW, Goodwin LR, Francom DM, Dieken FP, Kombian SB, Reiffenstein R. Dithiothreitol liberates non-acid labile sulfide from brain tissue of H₂S-poisoned animals. *Arch Toxicol* 1990;64(8):650–5.
- [147] Steinmann P, Shotyky W. Ion chromatography of organic-rich natural waters from peatlands IV. Dissolved free sulfide and acid-volatile sulfur. *J Chromatogr A* 1995;706(1–2):287–92.
- [148] Ditrói T, Nagy A, Martinelli D, Rosta A, Kožich V, Nagy P. Comprehensive analysis of how experimental parameters affect H₂S measurements by the monobromobimane method. *Free Radical Biol Med* 2019;136:146–58.
- [149] Hine C, Zhu Y, Hollenberg AN, Mitchell JR. Dietary and endocrine regulation of endogenous hydrogen sulfide production: implications for longevity. *Antioxid Redox Signal* 2018;28(16):1483–502.
- [150] Funazo K, Tanaka M, Morita K, Kamino M, Shono T, Wu H-L. Pentafluorobenzyl p-toluenesulphonate as a new derivatizing reagent for gas chromatographic determination of anions. *J Chromatogr A* 1985;346:215–25.
- [151] Kimura K, Hasegawa M, Matsubara K, Maseda C, Kagawa M, Takahashi S, Tanabe K-i. A fatal disaster case based on exposure to hydrogen sulfide—an estimation of the hydrogen sulfide concentration at the scene. *Forensic Sci Int* 1994;66(2):111–6.
- [152] Ali SE, Farag MA, Holvoet P, Hanafi RS, Gad MZ. A Comparative Metabolomics Approach Reveals Early Biomarkers for Metabolic Response to Acute Myocardial Infarction. *Sci Rep* 2016;6(1):36359.
- [153] Tan B, Jin S, Sun J, Gu Z, Sun X, Zhu Y, et al. New method for quantification of gas transmitter hydrogen sulfide in biological matrices by LC-MS/MS. *Sci Rep* 2017;7:46278.
- [154] Jin S, Tan B, Teng X, Meng R, Jiao X, Tian D, et al. Diurnal fluctuations in plasma hydrogen sulfide of the mice. *Front Pharmacol* 2017;8:682.
- [155] Mason J, Cardin C, Dennehy A. The role of sulphide and sulphide oxidation in the copper molybdenum antagonism in rats and guinea pigs. *Res Vet Sci* 1978;24(1):104–8.
- [156] Khan S, Morris G, Hidirolou M. Rapid estimation of sulfide in rumen and blood with a sulfide-specific ion electrode. *Microchem J* 1980;25(3):388–95.
- [157] Zhao W, Zhang J, Lu Y, Wang R. The vasorelaxant effect of H₂S as a novel endogenous gaseous KATP channel opener. *The EMBO Journal* 2001;20(21):6008–16.
- [158] Chen Y-H, Yao W-Z, Geng B, Ding Y-L, Lu M, Zhao M-W, et al. Endogenous Hydrogen Sulfide in Patients With COPD. *Chest* 2005;128(5):3205–11.
- [159] Olson KR. A Practical Look at the Chemistry and Biology of Hydrogen Sulfide. *Antioxid Redox Signal* 2011;17(1):32–44.
- [160] Li G, Polk BJ, Meazell LA, Hatchett DW. ISE Analysis of Hydrogen Sulfide in Cigarette Smoke. *J Chem Educ* 2000;77(8):1049.
- [161] Ri K, Kim S, Paek H, Hong C, Jon M. Determination of sulfide at screen-printed electrode modified with ferricyanide-doped partially quaternized poly (4-vinylpyridine). *J Electroanal Chem* 2019;853:113540.
- [162] Atta NF, Galal A, Mark HB, Yu T, Bishop PL. Conducting polymer ion sensor electrodes—III. Potentiometric sulfide ion selective electrode. *Talanta* 1998;47(4):987–99.
- [163] Kraus DW, Doeller JE. Sulfide consumption by mussel gill mitochondria is not strictly tied to oxygen reduction: measurements using a novel polarographic sulfide sensor. *J Exp Biol* 2004;207(21):3667–79.
- [164] Doeller JE, Isbell TS, Benavides G, Koenitzer J, Patel H, Patel RP, et al. Polarographic measurement of hydrogen sulfide production and consumption by mammalian tissues. *Anal Biochem* 2005;341(1):40–51.
- [165] Sun W, Fan J, Hu C, Cao J, Zhang H, Xiong X, et al. A two-photon fluorescent probe with near-infrared emission for hydrogen sulfide imaging in biosystems. *Chem Commun* 2013;49(37):3890–2.
- [166] Hong J, Zhou E, Gong S, Feng G. A red to near-infrared fluorescent probe featuring a super large Stokes shift for light-up detection of endogenous H₂S. *Dyes Pigment* 2019;160:787–93.
- [167] Zhang Y, Zhang B, Li Z, Wang L, Ren X, Ye Y. Endoplasmic reticulum targeted fluorescent probe for the detection of hydrogen sulfide based on a twist-blockage strategy. *Org Biomol Chem* 2019;17(38):8778–83.
- [168] Zhao X-j, Jiang Y-r, Li Y-t, Yang B-q, Liu C, Liu Z-h: A novel “turn-on” mitochondria-targeting near-infrared fluorescent probe for determination and bioimaging cellular hydrogen sulfide. *Spectrochim Acta Part A Mol Biomol Spectrosc* 2019;212:71–7.
- [169] Zou XJ, Ma YC, Guo LE, Liu WX, Liu MJ, Zou CG, et al. A lysosome-targeted fluorescent chemodosimeter for monitoring endogenous and exogenous hydrogen sulfide by in vivo imaging. *Chem Commun* 2014;50(89):13833–6.
- [170] Zhang H, Li M, Zhang C, Zhang G, Chao J, Shi L, et al. The design of hydrogen sulfide fluorescence probe based on dual nucleophilic reaction and its application for bioimaging. *Spectrochim Acta Part A Mol Biomol Spectrosc* 2019;207:150–5.
- [171] Palanisamy S, Lee L-Y, Wang Y-L, Chen Y-J, Chen C-Y, Wang Y-M. A water soluble and fast response fluorescent turn-on copper complex probe for H₂S detection in zebra fish. *Talanta* 2016;147:445–52.
- [172] Li X, Gong Y, Wu K, Liang SH, Cao J, Yang B, et al. A highly sensitive and water soluble fluorescent probe for rapid detection of hydrogen sulfide in living cells. *RSC Adv* 2014;4(68):36106–9.
- [173] Fu H, Duan X. Highly sensitive and colorimetric detection of hydrogen sulphide by in situ formation of Ag₂S@Ag nanoparticles in polyelectrolyte multilayer film. *RSC Adv* 2015;5(5):3508–11.
- [174] Zhao L, Zhao L, Miao Y, Liu C, Zhang C. A Colorimetric Sensor for the Highly Selective Detection of Sulfide and 1,4-Dithiothreitol Based on the In Situ Formation of Silver Nanoparticles Using Dopamine. *Sensors* 2017;17(3):626.
- [175] Tang S, Qi T, Xia D, Xu M, Xu M, Zhu A, et al. Smartphone Nanocolorimetric Determination of Hydrogen Sulfide in Biosamples after Silver-Gold Core-Shell Nanoparticle-Based Headspace Single-Drop Microextraction. *Anal Chem* 2019;91(9):5888–95.
- [176] Hao J, Xiong B, Cheng X, He Y, Yeung ES. High-Throughput Sulfide Sensing with Colorimetric Analysis of Single Au–Ag Core-Shell Nanoparticles. *Anal Chem* 2014;86(10):4663–7.
- [177] Chen Z, Chen C, Huang H, Luo F, Guo L, Zhang L, et al. Target-Induced Horseradish Peroxidase Deactivation for Multicolor Colorimetric Assay of Hydrogen Sulfide in Rat Brain Microdialysis. *Anal Chem* 2018;90(10):6222–8.
- [178] Varlet V, Giuliani N, Palmiere C, Maujean G, Augsburger M. Hydrogen sulfide measurement by headspace-gas chromatography-mass spectrometry (HS-GC-MS): Application to gaseous samples and gas dissolved in muscle. *J Anal Toxicol* 2014;39(1):52–7.
- [179] Vitvitsky V, Banerjee R: H₂S analysis in biological samples using gas chromatography with sulfur chemiluminescence detection. In: *Methods in enzymology*. vol. 554: Elsevier; 2015: 111–123.